

Agilent 4291B

RF Impedance/Material Analyzer

Data Sheet

Discontinued Product Information — For Support Reference Only —

Information herein, may refer to products/services no longer supported. We regret any inconvenience caused by obsolete information. For the latest information on Agilent's test and measurement products go to: www.agilent.com/find/products

In the US, call Agilent Technologies at 1-800-829-4444 (any weekday between 8am-5pm in any U.S. time zone)

World-wide Agilent sales office contact information is available at: www.agilent.com/find/contactus

Overview

Specifications describe the instrument's warranted performance over the temperature range of $0^{\circ}\mathrm{C}$ to $40^{\circ}\mathrm{C}$ (except as noted). Supplemental characteristics are intended to provide information that is useful in applying the instrument by giving nonwarranted performance parameters.

These are denoted as "typical," "nominal," or "approximate." Warm-up time must be greater than or equal to 30 minutes after power on for all specifications. Specifications of the stimulus characteristics and measurement accuracy are defined at the tip of APC-7 connector on the test head connected to the instrument.

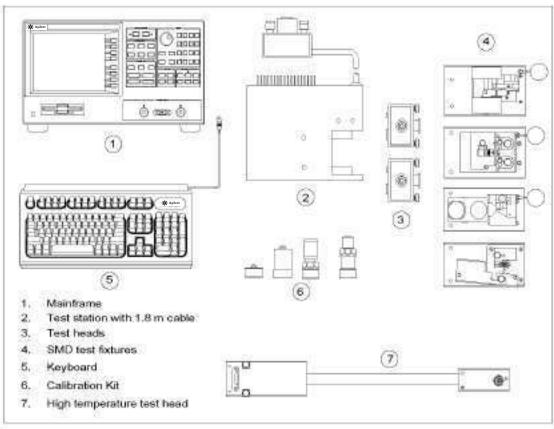


Figure 1-1



$\label{eq:measurement Parameters} \begin{subarray}{l} \textbf{Measurement Parameters} \\ \textbf{IZ} ,~\theta_z,~ Y ,~\theta_y,~R,~X,~G,~B,~C_p,~C_s,~L_p,~L_s,~R_p,~R_s,~D,~Q,~ \Gamma ,~\theta_y,~\Gamma_x,~\Gamma_y \end{subarray}$
$\begin{array}{c} \textbf{Stimulus Characteristics} \\ \textbf{Frequency Characteristics} \\ \textbf{Operating frequency} & 1 \ \text{MHz to } 1.8 \ \text{GHz} \\ \textbf{Frequency resolution} & 1 \ \text{mHz} \\ \textbf{Frequency reference} \\ \textbf{Accuracy} \\ @ \ 23\pm5^{\circ}\text{C} & < \pm 10 \ \text{ppm} \\ \end{array}$
Precision frequency reference (Option 1D5) Accuracy @ 0° C to 40° C
Source Characteristics
$\begin{tabular}{lll} \textbf{OSC level} \\ \textbf{Voltage range} \\ @ 1 \ MHz \le Frequency \le 1 \ GHz \ (When terminal is open) & 0.2 \ mV_{rms} \ to \ 1 \ V_{rms} \\ @ 1 \ GHz < Frequency \le 1.8 \ GHz \ (When terminal is open) & 0.2 \ mV_{rms} \ to \ 0.5 \ V_{rms} \\ \end{tabular}$
$\begin{tabular}{lll} \textbf{Current range} \\ @ 1 \ MHz \le Frequency \le 1 \ GHz \ (When terminal is shorted). & 4 \ \mu A_{rms} \ to \ 20 \ mA_{rms} \\ @ 1 \ GHz < Frequency \le 1.8 \ GHz \ (When terminal is shorted). & 4 \ \mu A_{rms} \ to \ 10 \ mA_{rms} \\ \end{tabular}$
Power range @ 1 MHz \leq Frequency \leq 1 GHz (When terminating with 50 Ω)
$ \begin{array}{llllllllllllllllllllllllllllllllllll$
$\begin{array}{lll} 22 \text{ mV}_{rms} < V_{OSC} \le 70 \text{ mV}_{rms} & 0.2 \text{ mV} \\ 7 \text{ mV}_{rms} < V_{OSC} \le 22 \text{ mV}_{rms} & 0.05 \text{ mV} \\ 2.2 \text{ mV}_{rms} < V_{OSC} \le 7 \text{ mV}_{rms} & 0.02 \text{ mV} \\ 0.7 \text{ mV}_{rms} < V_{OSC} \le 2.2 \text{ mV}_{rms} & 0.005 \text{ mV} \\ 0.2 \text{ mV}_{rms} \le V_{OSC} \le 0.7 \text{ mV}_{rms} & 0.002 \text{ mV} \end{array}$

$\begin{array}{llllllllllllllllllllllllllllllllllll$
where, $ \begin{array}{lllllllllllllllllllllllllllllllllll$
@ 250 mV _{rms} > V _{OSC} \geq 2.5 mV _{rms}
Definition of OSC level • Voltage level: $2 \times$ voltage level across the $50~\Omega$ which is connected to the output terminal (This level is approximately equal to the level when a terminal is open.) • Current level: $2 \times$ current level through the $50~\Omega$ which is connected to the output terminal (This level is approximately equal to the level when a terminal is shorted.) • Power level: when terminating with $50~\Omega$
OSC level accuracy ½ of specification value (typical) Connector APC-7 Output impedance 50 Ω (Nominal value) DC bias (Option 001) 0 to ±40V DC current level 20 μ A to 100 mA and -20 μ A to -100 mA DC level resolution 1 mV, 20 μ A DC level accuracy $0.22 \pm 5.9 C$

Level monitor

Monitor parameters	OSC level (voltage, current), DC bias (voltage, current)
Monitor accuracy	
OSC level	Same as OSC level accuracy (typical)
DC bias	. Twice as bad as specifications of dc level accuracy (typical)

Sweep Characteristics

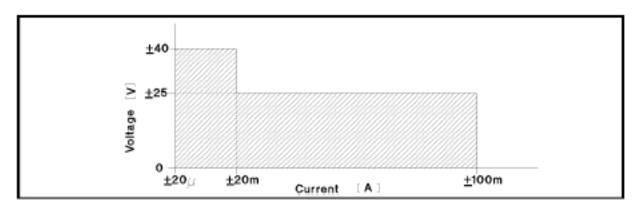


Figure 1-2. DC Voltage and Current Level Range (Typical)

Sweep parameters Frequency, OSC level (voltage), DC bias voltage/current Sweep setup Start Stop, or Center Span Sweep type
Frequency sweep Linear, Log, Zero-span, List Other sweep parameters Linear, Log, Zero-span
Sweep mode
Sweep direction
AC level, DC bias (voltage and current)
Number of measurement points
Averaging
Delay time
Measurement circuit mode
Calibration/Compensation
$\textbf{Calibration function} Open/Short/50~\Omega~calibration, Low~loss~calibration$

Measurement Accuracy

Conditions of accuracy specifications

- Open/Short/50 Ω calibration must be done. Calibration ON.
- Averaging (on point) factor is larger than 32 at which calibration is done if Cal points is set to USER DEF.
- Measurement points are same as the calibration points.
- Environmental temperature is within ±5°C of temperature at which calibration is done, and within l3°C to 33°C. Beyond this environmental temperature condition, accuracy is twice as bad as specified.

$ \textbf{Z} , \textbf{Y} \textbf{Accuracy}\ldots\pm(E_a+E_b)[\%]$
The illustrations of $ Z $ and $ Y $ accuracy are shown in Figures l-3 to 1-6.
θ Accuracy $\qquad \qquad \pm \frac{(E_a + E_b)}{100} [rad]$
L, C, X, B Accuracy $ \begin{array}{ccccccccccccccccccccccccccccccccccc$
$ @ D_x tan \left(\frac{E_a + E_b}{100}\right) < 1 $ $ = \frac{(1 + D_x^2)tan \left(\frac{E_a + E_b}{100}\right)}{1 \mp D_x tan \left(\frac{E_a + E_b}{100}\right)} $
Especially, @ $D_x \le 0.1$.
$ \begin{array}{c} \textbf{0 Accuracy } (\Delta \textbf{0}) \\ @ \mid Q_x tan \ (\frac{E_a + E_b}{100}) \mid \leq 1. \end{array} \\ & \pm \frac{(1 + Q_x^2) tan \ (\frac{E_a + E_b}{100})}{(1 \mp Q_x) tan \ (\frac{E_a + E_b}{100})} \\ \end{array} $
Especially, @ $\frac{10}{(E_a + E_b)} \ge Q_x \ge 10$ $\pm Q_x^2 \frac{(E_a + E_b)}{100}$
Where, $ \begin{array}{l} \textbf{D}_{\textbf{x}} : \text{Measured vaulue of D} \\ \textbf{E}_{\textbf{a}} : \text{depends on measurement frequency as follows:} \\ @ 1 \text{ MHz} \le \text{Frequency} \le 100 \text{ MHz} & 0.6 \\ @ 100 \text{ MHz} < \text{Frequency} \le 500 \text{ MHz} & 0.8 \\ @ 500 \text{ MHz} < \text{Frequency} \le 1000 \text{ MHz} & 1.2 \\ @ 1000 \text{ MHz} < \text{Frequency} \le 1800 \text{ MHz} & 2.0 \\ \textbf{E}_{\textbf{b}} = (Z_{\textbf{s}}/ Z_{\textbf{x}} + Y_{\textbf{o}} Z_{\textbf{x}} \times 100 \\ \textbf{O}_{\textbf{x}} : \text{Measured value of } Q \\ \textbf{Z}_{\textbf{x}} : \text{impedance measurement value } [\Omega] \\ \textbf{Z}_{\textbf{s}} \text{ and } \textbf{Y}_{\textbf{o}} \text{ depend on number of point averaging } (N_{av}), \text{ OSC level } (V_{OSC}), \text{ impedance measurement value } (Z_{\textbf{x}}) \text{ and the test head used as follows:} \\ \end{array} $

Table 1-1. Z_s and Y_o When High Impedance Test Head Is Used

Measurement Conditions

Number of Point Averaging (N _{av})	OSC Signal Level (V_{osc})	Meas. Impedance (Z_x)	$Z_{S}\left[\Omega ight]$	Y _o [S]
	V _{osc} < 0.02V	-	$\frac{0.02}{V_{osc}} \times (0.2 + 0.001 \times f_{[MHz]})$	$\frac{0.02}{V_{osc}}$ x (5 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz])
$1 \le N_{av} \le 7$	$0.02V \le V_{osc} < 0.12V$	_	0.2 + 0.001 x f _[MHz]	5 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz]
	$0.12V \le V_{osc}$	Z _x ≥ 500 Ω	0.2 + 0.001 x f _[MHz]	5 x 10 ⁻⁶ + 2 x 10 ⁻⁷ x f _[MHz]
		Z_x < 500 Ω	0.2 + 0.001 x f _[MHz]	2 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz]
	V _{osc} < 0.02V		$\frac{0.02}{V_{osc}} \times (0.1 + 5 \times 10^{-4} \times f_{[MHz]})$	$\frac{0.02}{V_{osc}}$ x (2 x 10 ⁻⁵ + 1 x 10 ⁻⁷ x f _[MHz]
$N_{av} \geq 8$	$0.02V \le V_{osc} < 0.12V$		0.1 + 5 x 10 ⁻⁴ x f _[MHz]	2 x 10 ⁻⁵ + 1 x 10 ⁻⁷ x f _[MHz]
	$0.12V \le V_{\rm osc}$	Z _x ≥ 500 Ω	0.1 + 5 x 10 ⁻⁴ x f _[MHz]	2 x 10 ⁻⁶ + 1 x 10 ⁻⁷ x f _[MHz]
		Z_x < 500 Ω	0.1 + 5 x 10 ⁻⁴ x f _[MHz]	7 x 10 ⁻⁶ + 1 x 10 ⁻⁷ x f [MHz]

Table 1-2. Z_{s} and Y_{o} When Low Impedance Test Head Is Used

Measurement Conditions

Number of Point Averaging (N _{av})	OSC Signal Level (V_{osc})	Meas. Impedance (Z_x)	$Z_{\$}\left[\Omega ight]$	Y _o [S]
	$V_{\rm osc} < 0.02V$	-	$\frac{0.02}{V_{osc}}$ x (0.1 + 0.001 x f _[MHz])	$\frac{0.02}{V_{osc}}$ x (1 x 10 ⁻⁴ + 2 x 10 ⁻⁷ x f _[MHz])
$1 \leq N_{av} \leq 7$	$0.02V \le V_{osc} < 0.12V$		0.1 + 0.001 x f _[MHz]	1 x 10 ⁻⁴ + 2 x 10 ⁻⁷ x f _[MHz]
	0.12V ≤ V _{osc}	$Z_x \le 5 \Omega$	0.01 + 0.001 x f _[MHz]	1 x 10 ⁻⁴ + 2 x 10 ⁻⁷ x f _[MHz]
		$Z_x > 5 \Omega$	0.05 + 0.001 x f _[MHz]	1 x 10 ⁻⁴ + 2 x 10 ⁻⁷ x f _[MHz]
	V _{osc} < 0.02V	_	$\frac{0.02}{V_{osc}} \times (0.05 + 5 \times 10^{-4} \times f_{[MHz]})$	$\frac{0.02}{V_{osc}}$ x (3 x 10 ⁻⁵ + 1 x 10 ⁻⁷ x f _[MHz]
$N_{\text{av}} \geq 8$	$0.02V \le V_{osc} < 0.12V$		0.05 + 5 x 10 ⁻⁴ x f _[MHz]	3 x 10 ⁻⁵ + 1 x 10 ⁻⁷ x f _[MHz]
	0.12V ≤ V _{osc}	$Z_x \leq 5 \Omega$	0.01 + 5 x 10 ⁻⁴ x f _[MHz]	3 x 10 ⁻⁵ + 1 x 10 ⁻⁷ x f _[MHz]
		$Z_x > 5 \Omega$	0.02 + 5 x 10 ⁻⁴ x f _[MHz]	3 x 10 ⁻⁵ + 1 x 10 ⁻⁷ x f [MHz]

At the following frequency points, instrument spurious characteristics could occasionally cause measurement errors to exceed specified value because of instrument spurious characteristics.

10.71 MHz 514.645 MHz 17.24 MHz 686.19333 MHz 21.42 MHz 1029.29 MHz 42.84 MHz 1327.38666 MHz

See "EMC" under "Others" in "General Characteristics."

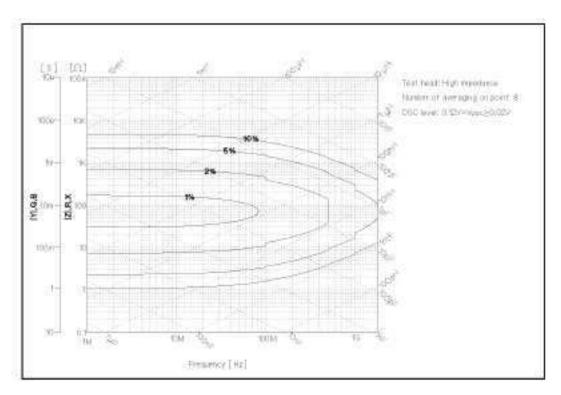


Figure 1-3. Impedance Measurement Accuracy Using High Impedance Test Head (@ Low OSC Level)

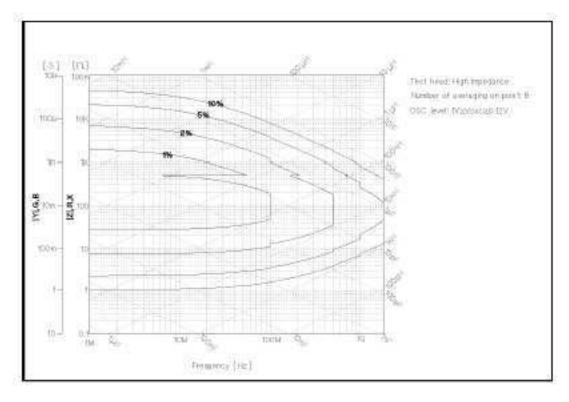


Figure 1-4. Impedance Measurement Accuracy Using High Impedance Test Head (@ High OSC Level)

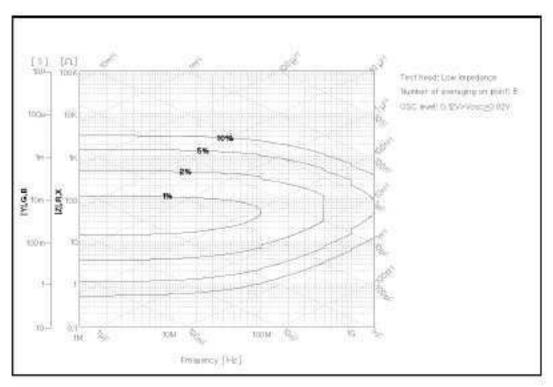


Figure 1-5. Impedance Measurement Accuracy Using Low Impedance Test Head (@ Low OSC Level)

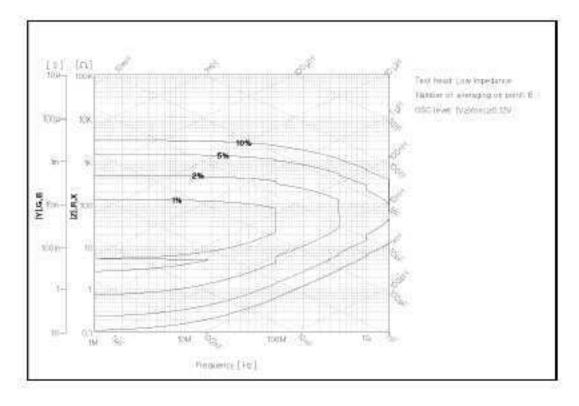


Figure 1-6. Impedance Measurement Accuracy Using Low Impedance Test Head (@ High OSC Level)

Typical measurement accuracy when open/short/50 Ω /low-loss-capaciter calibration is done

Conditions

- Averaging on point factor is larger than 32 at which calibration is done.
- Cal Points is set to USER DEF.
- Environmental temperature is within ±5°C of temperature at which calibration is done, and within 13°C to 33°C. Beyond this environmental temperature condition, accuracy is twice as bad as specified.

Where,

 $\mathbf{D}_{\mathbf{X}}$: Actual D value of DUT

 \textbf{E}_{a} , \textbf{E}_{b} : are as same as E_{a} and E_{b} of the measurement accuracy when OPEN/SHORT/50 Ω calbration is done.

$$\mathbf{E_c} = 0.06 + 0.14 \times \frac{F}{1800}$$
 (Typical)

F: measurement frequency [MHz]

 $\mathbf{Q}_{\mathbf{x}}$: Actual Q value of DUT

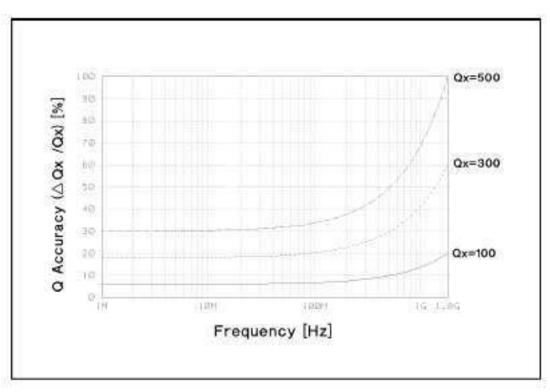


Figure 1-7. Typical measurement accuracy when open/short/50 Ω /low-loss-capaciter calibration is done

Specification for Option 013 and 014 High Temperature Test Heads Frequency Characteristics
Operating frequency
Source Characteristics OSC level Voltage Range
OSC level resolution
AC voltage resolution
$ @ 110 \text{ mV}_{\text{rms}} < \text{V}_{\text{OSC}} \le 500 \text{ mV}_{\text{rms}}. \qquad \qquad 2 \text{ mV} $
@ 11 mV _{rms} $<$ V _{OSC} \le 110 mV _{rms}
@ 1.1 mV _{rms} $<$ V _{OSC} \le 11 mV _{rms}
$ @ 0.2 \text{ mV}_{\text{rms}} \leq \text{V}_{\text{OSC}} \leq 1.1 \text{ mV}_{\text{rms}} \dots 2 \mu\text{V} $
AC current resolution
@ $2.75 \text{ mA}_{\text{rms}} < I_{\text{OSC}} \le 12.5 \text{ mA}_{\text{rms}} \dots 50 \mu\text{A}$
@ $0.275 \text{ mA}_{\text{rms}} < I_{\text{OSC}} \le 2.75 \text{ mA}_{\text{rms}}$
@ $27.5 \ \mu A_{rms} < I_{OSC} \le 275 \ \mu A_{rms}$
@ 5 μ A \leq I _{OSC} \leq 27.5 μ A
AC power resolution
$ @ -66.1 \text{ dBm} \le P_{OSC} \le 1.9 \text{ dBm} \dots 0.2 \text{ dBm max} $
OSC level accuracy
@ 1 MHz \leq Frequency \leq 1 GHz, $V_{OSC} \leq$ 0.25 V_{rms} ($I_{OSC} \leq$ 6.3 mA, $P_{OSC} \leq$ -4.1 dBm)
A + B + $8[dB] \times frequency[MHz]dB$ 1800
Where,
A depends on temperature conditions as follows:
within referenced to $23\pm5^{\circ}\mathrm{C}$
B depends on OSC level as follows:
$ @ 0.5 \text{ V}_{rms} \ge \text{V}_{OSC} \ge 120 \text{ mV}_{rms} \dots 0 \text{ dB} $
$(12.5 \text{ mA}_{\text{rms}} \ge I_{\text{OSC}} \ge 3\text{mA}_{\text{rms}})$
$(1.9 \text{ dBm} \ge P_{OSC} \ge -10 \text{ dBm})$
@ 120 mV _{rms} > V _{OSC} \geq 1.2 mV _{rms}
(3 mA _{rms} > $I_{OSC} \ge 30 \mu A_{rms}$)
$(3 \text{ mA}_{\text{rms}})^{-10 \text{ SC}} \ge 30 \mu\text{A}_{\text{rms}})$ $(-10 \text{ dBm} > P_{\text{OSC}} \ge -50 \text{ dBm})$
$(-10 \text{ dDiff} > 1 \text{ 080 \ge -50 \text{ dDiff})$
@ $1.2 \text{ mV}_{rms} > V_{OSC} \ge 0.2 \text{ mV}_{rms}$
$(30 \ \mu A_{rms} > I_{OSC} \ge 0.2 \ \text{m} v_{rms})$
$(-50 \text{ dBm} > P_{OSC} \ge -66.1 \text{ dBm})$
\sim 0 dBM \sim 1 $_{\rm OSC} \simeq$ -00.1 dBM) Output impedance
Level Monitor
Monitor accuracy
OSC level Same as OSC level accuracy (typical)
DC bias
Do mas I wice as pad as specifications of defever accuracy (typical)

Basic Measurement Accuracy

Conditions of accuracy specifications

- OPEN/SHORT/50 Ω calibration must be done. Calibration ON.
- Averaging (on point) factor must be larger than 32 at which calibration is done.
- Measurement points are same as the calibration points.
- Environmental temperature is within ±5°C of temperature at which calibration is done, and within 13°C to 33°C. Beyond this environmental temperature condition, and within 0°C to 40°C, accuracy is twice as bad as specified.
- Bending cable should be smooth and the bending angle is less than 30°.
- Cable position should be kept in the same position after calibration measurement.
- OSC level must be same as level at which calibration is done.
- OSC level is less than or equal to 0.25 V, or OSC level is greater than 0.25 V and frequency range is within 1 MHz to 1 GHz.

$\begin{tabular}{lllllllllllllllllllllllllllllllllll$
θ Accuracy $\qquad \qquad \pm \frac{(E_a + E_b)}{100} [rad]$
Where,
\mathbf{E}_{a} : depends on measurement frequency as follows:
@ 1 MHz ≤ frequency ≤ 100 MHz
@ 100 MHz < frequency ≤ 500 MHz
@ 500 MHz < frequency ≤ 1 GHz
@ 1 GHz < frequency ≤ 1.8 GHz
$\mathbf{E_b} = (\mathbf{Z_s/Z_x} + \mathbf{Y_oZ_x}) \times 100 [\%]$
$\mathbf{Z_s}$ and $\mathbf{Y_o}$ depend on number of point averaging (N_{av}) and OSC level (V_{osc}) as follows:
7.: Impedance measurement value [O]

Table 1-3. Z_{s} and Y_{o} When High Impedance Test Head Is Used

Measurement Conditions

Number of Point Averaging (N _{av})	OSC Signal Level (V _{osc}) ¹	$Z_{S}\left[\Omega ight]$	Y _o [S]
	V _{osc} < 0.02	$\frac{0.02}{V_{osc}} \times (0.2 + 0.001 \times f_{[MHz]})$	$\frac{0.02}{V_{osc}}$ x (5 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz])
$1 \leq N_{av} \! \leq \! 7$	$0.02V \le V_{osc} < 0.12$	0.2 + 0.001 x f _[MHz]	5 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz]
	$0.12V \le V_{osc}$	0.2 + 0.001 x f _[MHz]	3 x 10 ⁻⁶ + 2 x 10 ⁻⁷ x f _[MHz]
	V _{osc} < 0.02	$\frac{0.02}{V_{osc}} \times (0.1 + 0.001 \times f_{[MHz]})$	$\frac{0.02}{V_{osc}}$ x (2 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz])
$8 < N_{av}$	$0.02V \le V_{osc} < 0.12$	0.1 + 0.001 x f _[MHz]	2 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz]
	$0.12V \le V_{osc}$	0.1 + 0.001 x f _[MHz]	2 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz]

 $^{1.~}V_{osc} = 0.12V \equiv I_{osc} = 3~mA \equiv P_{OSC} = -10~dBm,~V_{osc} = 0.02V \equiv I_{osc} = 0.5~mA \equiv P_{osc} = -26~dBm$

Table 1-4. Z_s and Y_o When Low Impedance Test Head Is Used

Measurement Conditions

Number of Point Averaging (N _{av})	OSC Signal Level (V _{osc})¹	$Z_{S}\left[\Omega ight]$	Y _o [S]
	V _{osc} < 0.02	$\frac{0.02}{V_{osc}} \times (0.1 + 0.001 \times f_{[MHz]})$	$\frac{0.02}{V_{osc}}$ x (1 x 10 ⁻⁴ + 2 x 10 ⁻⁷ x f _[MHz])
$1 \le N_{av} \le 7$	$0.02V \le V_{osc} < 0.12$	0.1 + 0.001 x f _[MHz]	1 x 10 ⁻⁴ + 2 x 10 ⁻⁷ x f _[MHz]
	$0.12V \le V_{osc}$	0.05 + 0.001 x f _[MHz]	$1 \times 10^{-4} + 2 \times 10^{-7} \times f_{[MHz]}$
	V _{osc} < 0.02	$\frac{0.02}{V_{\rm osc}} \times (0.05 + 0.001 \times f_{\rm [MHz]})$	$\frac{0.02}{V_{osc}}$ x (3 x 10 ⁻⁵ + 2 x 10 ⁻⁷ x f _[MHz])
$8 < N_{av}$	$0.02V \le V_{\rm osc} < 0.12$	$0.05 + 0.001 \times f_{[MHz]}$	$3 \times 10^{-5} + 2 \times 10^{-7} \times f_{[MHz]}$
	0.12V ≤ V _{osc}	0.03 + 0.001 x f _[MHz]	$3 \times 10^{-5} + 2 \times 10^{-7} \times f_{[MHz]}$

 $^{1.~}V_{osc} = 0.12V \equiv I_{osc} = 3~mA \equiv P_{OSC} = -10~dBm,~V_{osc} = 0.02V \equiv I_{osc} = 0.5~mA \equiv P_{osc} = -26~dBm$

At the following frequency points, instrument spurious characteristics could occasionally cause measurement errors to exceed specified value because of instrument spurious characteristics.

 10.71 MHz
 17.24 MHz
 21.42 MHz
 42.84 MHz

 514.645 MHz
 686.19333 MHz
 1029.29 MHz
 1327.38666 MHz

See "EMC" under "Others" in "General Characteristics."

The excessive vibration and shock could occasionally cause measurement errors to exceed specified values.

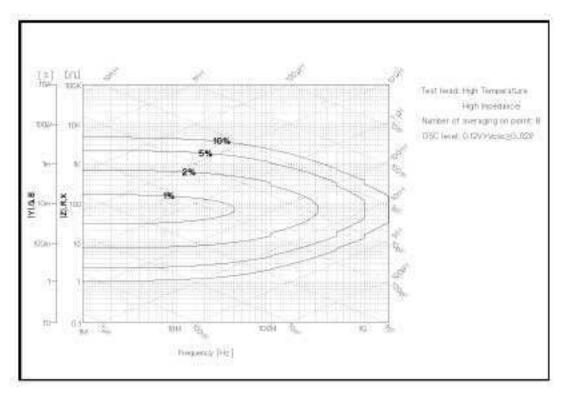


Figure 1-8. Impedance Measurement Accuracy Using High Temperature High Impedance Test Head (@ Low OSC Level)

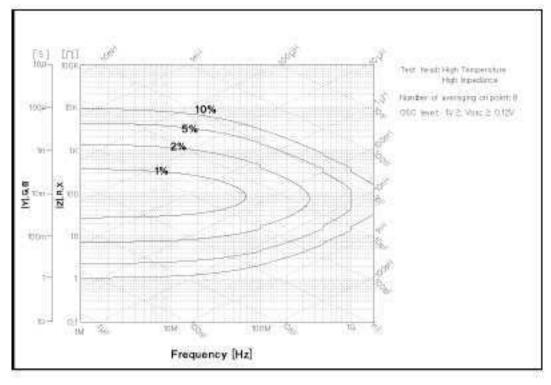


Figure 1-9. Impedance Measurement Accuracy Using High Temperature High Impedance Test Head (@ High OSC Level)

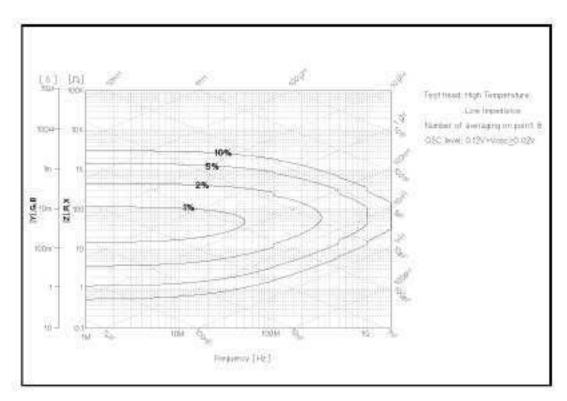


Figure 1-10. Impedance Measurement Accuracy Using High Temperature Low Impedance Test Head (@ Low OSC Level)

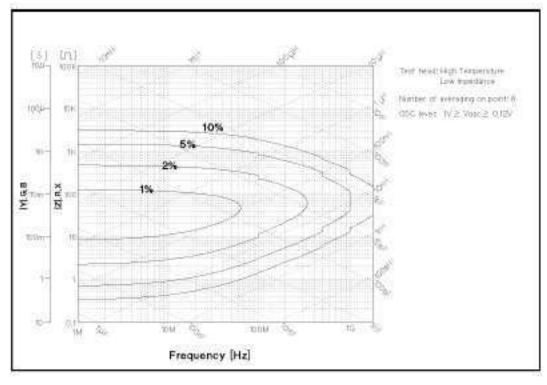


Figure 1-11. Impedance Measurement Accuracy Using High Temperature Low Impedance Test Head (@ High OSC Level)

Typical Effects of Temperature Drift on Measurement Accuracy

When environmental temperature exceeds ± 5 °C of temperature at which calibration is done, add the following measurement error.

Conditions of typical effects of temperature drift

- Environment temperature of a test head is within -55°C to 0°C or 40°C to 200°C.
- Environment temperature of the mainframe is within ±5°C of temperature at which calibration is done, and within 0°C to 40°C.
- Other conditions are as same as the conditions of the basic measurement accuracy of Option 013/014.

Where,

$$\mathbf{E_{a2}} = (\Delta A_1 \Delta T + \Delta A_2) \times 10^8$$

$$\mathbf{E_{b2}} = (Z_{s2}/Z_x + Y_{o2}Z_x) \times 100$$

 ΔA_1 is the effect of temperature drift on the impedance measurement value as follows:

 $(50 + 300 \times f)$ [ppm/°C] (typical)

 ΔA_2 is the hysterisiss of the effect of temperature drift on the impedance measurement value as follows:

$$\frac{\Delta A_1 \Delta T}{3}$$
 [ppm] (typical)

f: Measurement Frequency [GHz]

ΔT: Difference of temperature between measurement condition and calibration measurement condition. [°C]

$$\mathbf{Y_{o2}} = (\Delta \mathbf{Y}_{o1} \Delta \mathbf{T} + \Delta \mathbf{Y}_{o2}) \times 10^{-6} [S]$$

$$\mathbf{Z}_{s2} = (\Delta \mathbf{Z}_{s1} \Delta \mathbf{T} + \Delta \mathbf{Z}_{s2}) \times 10^{-3} [\Omega]$$

 $\mathbf{Z}_{\mathbf{x}}$: Impedance measurement value $[\Omega]$

 Y_{01} is the temperature coefficient for OPEN residual as follows:

- @ High Temperature High Impedance Test Head is used $(0.2 + 8 \times f^2)$ [μ S/°C] (typical)
- @ High Temperature Low Impedance Test Head is used (1 + 30 \times f) [μ S/ $^{\circ}$ C] (typical)

 $\mathbf{Y}_{\mathbf{02}}$ is the hysterisis of the OPEN residual as follows: $\frac{\Delta Y_{01}\Delta T}{3}$ [μ S/°C](typical)

 ΔZ_{s1} is the temperature coefficient for SHORT residual as follows:

- @ High Temperature High Impedance Test Head is used $(4 + 50 \times f)$ [m Ω °C] (typical)

 ΔZ_{s2} is the hysterisis of the SHORT residual as follows: $\frac{\Delta Z_{s1}\Delta T}{3}$ [m Ω /°C](typical)

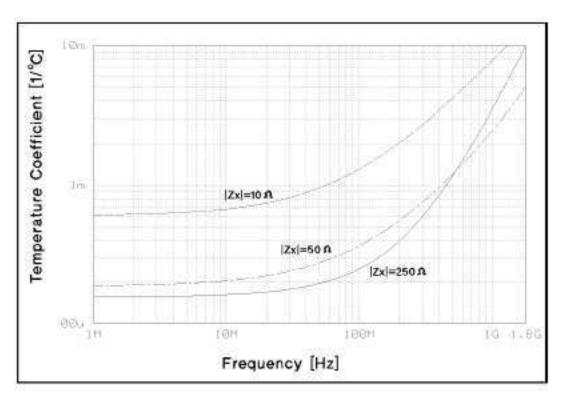


Figure 1-12. Typical Frequency Characteristics of Temperature Coefficient Using High Temperature High Impedance Test Head

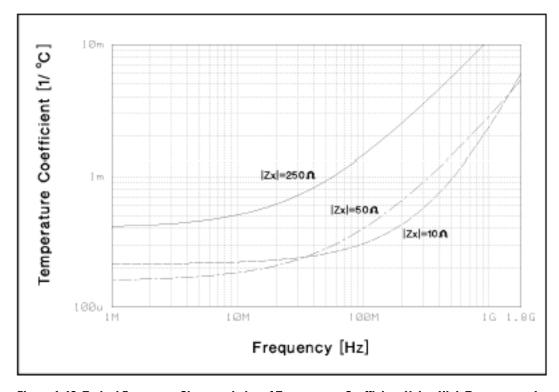


Figure 1-13. Typical Frequency Characteristics of Temperature Coefficient Using High Temperature Low Impedance Test Head

Operation Conditions of the Test Head

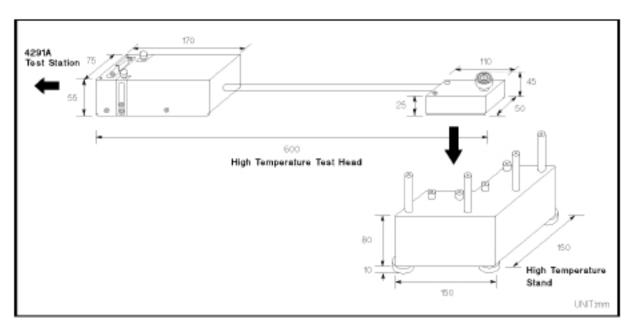


Figure 1-14. Dimensions of High Temperature Test Head

Display
LCD
Type/size
Resolution
Effective Display Area
Number of display channels $\dots \dots \dots$
Format
Number of traces
For measurement
For memory
Data math functions
$\operatorname{gain} imes \operatorname{memory}$ – offset
$\operatorname{gain} imes (\operatorname{data} - \operatorname{memory}) - \operatorname{offset}$
$\operatorname{gain} imes (\operatorname{data} + \operatorname{memory})$ – offset
$gain \times (data/memory)$ – offset
$\operatorname{gain} \times (\operatorname{data} \times \operatorname{memory})$ – offset
Marker
Number of markers
Main marker
Sub-marker
Δ Marker
Data Storage
Type floppy disk drive, Volatile memory disk
Capacity
floppy disk
Volatile memory disk, can be backed up by flash memory
Disk formatLIF, DOS
GPIB
Interface IEEE 488.1-1987, IEC625
DC1, DT1, C1, C2, C3, C4, C11, E2
Numeric Data Transfer formats
32 and 64 bit IEEE 754 Floating point format,
DOS PC format (32 bit IEEE with byte order reversed)
Protocol IEEE 488.2-1987

Printer Parallel Port	
Interface	IEEE 1284 Centronics standard compliant
	HP PCL3 Printer Control Language
General Characteristics	
Input and Output Characteristics	
External reference input	
Frequency	
	> -6 dBm (typically)
Input impedance	$\ldots \ldots $
	BNC female
Internal Reference Output	
Frequency	10 MHz (nominal)
	$\ldots \ldots $
	BNC female
External trigger input	
Level	
	> 2μ s (typically)
	positive/negative selective
•	BNC female

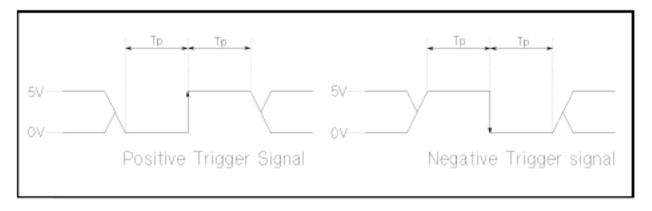


Figure 1-15. Trigger Signal

Operation Conditions
Temperature
Disk drive non-operating condition
Humidity
@ wet bulb temperature <29°C, without condensation
Disk drive non-operating condition 15 % to 95 % RH Disk drive operating condition 15 % to 80 % RH
Altitude
Warm-up time
Non-operation conditions
Temperature
@ wet bulb temperature <45°C, without condensation
Altitude
Others
EMC
Complies with IEC 1000-4-2 (1995) / EN 50082-1 (1992) : 4 kV CD, 8 kV AD
Complies with IEC 1000-4-4 (1995) / EN 50082-1 (1992) : 1 kV / Main, 0.5k V / Signal Line
Note: When tested at 3 V/m according to IEC 1000-4-3 (1995), the measurement accuracy will be within specifications over the full immunity test frequency range of 27 to 1000 MHz except when the analyzer frequency is identical to the transmitted interference signal test frequency.
Safety Complies with IEC 1010-1 (1990), Amendment 1 (1992) and Amendment 2 (1995).
Power requirements 90V to 132V, or 198V to 264V (automatically switched), 47 to 63 Hz, 300VA max
Weight
Mainframe
Test Station
Dimensions
$\begin{tabular}{lllllllllllllllllllllllllllllllllll$

External Program Run/Cont Input

Connector
Level
Keyboard connector mini-DII
I/O port

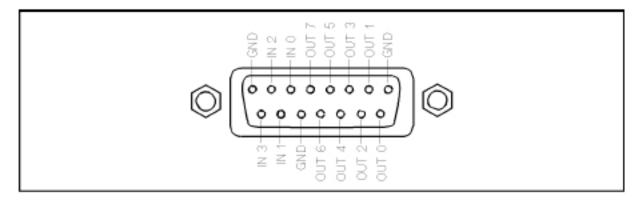


Figure 1-16. I/O Port Pin Assignment

Specifications for Option 1D5 High Stability Frequency Reference

Reference Oven Output

Frequency	 	 	10 MHz (nominal)
Level	 	 • • • • • • • • • • • • • • • •	0 dBm (typically)
Output Impedance	 	 	50Ω (nominal)
Connector	 	 	BNC female

Supplemental Characteristics for Option 002 Material Measurement

Measurement Frequency Range

Using the Agilent 16453A	1 MHz to 1.0 GHz (Typical)
Using the Agilent 16454A	1 MHz to 1.0 GHz (Typical)

Measurement Parameters

Permittivity parameters	$ \epsilon_{ m r} , \epsilon_{ m r}', \epsilon_{ m r}'', an$
Permeability parameters	$ \mu_{\rm r} , \mu_{\rm r}', \mu_{\rm r}'', an$

Typical Measurement Accuracy

Conditions of accuracy characteristics

- Use the High Z Test Head for permittivity measurement
- Use the Low Z Test Head for permeability measurement
- OPEN/SHORT/50 Ω calibration must be done. Calibration ON.
- Averaging (on point) factor is larger than 32 at which calibration is done if Cal points is set to USER DEF.
- Measurement points are same as the calibration points if Cal point is set to USER DEF.
- Environment temperature is within ±5°C of temperature at which calibration is done, and within 13°C to 33°C. Beyond this environmental temperature condition, accuracy is twice as bad as specified.

$$\epsilon_{\text{r}}^{\text{ '}}$$
 Accuracy $(\frac{\Delta\epsilon'_{rm}}{\epsilon'_{rm}})$

Where,

@ frequency ≤ 1 GHz

$$\mathbf{E_a} = 0.002 + \frac{0.0004}{f} \quad \frac{t}{\epsilon'_{\text{m}}} + 0.004f + \frac{0.1}{|1 - (13/\sqrt{\epsilon'_{\text{rm}}}/f)^2|} \text{ (Typical)}$$

@ frequency > 1 GHz

$$\textbf{E}_{\textbf{a}} = 0.002 + \frac{0.0004}{\textit{f}} \quad \frac{\textit{t}}{\textit{\epsilon'}_{m}} + 0.004\textit{f} + \frac{0.1}{|1 - (13/\sqrt{\textit{\epsilon'}_{rm}}/\textit{f})^{2}|} \text{(Typical)}$$

$$\mathbf{E_b} = \left(\frac{\Delta \varepsilon'_{\rm rm}}{\varepsilon'_{\rm rm}} \frac{1}{100} + \varepsilon'_{\rm rm} \frac{0.002}{t}\right) \ \tan\delta \ (\text{Typical})$$

f is measurement frequency [GHz]

t is thickness of MUT [mm]

 ϵ'_{rm} is measured value of ϵ'_{r}

tand is measured value of dielectric loss tangent

$$\text{@} \ \tan \delta < 0.1 \ldots \qquad \qquad 4 + \frac{25}{F\mu'_{rm}} + F\mu'_{rm} (1 + \frac{15}{F\mu'_{rm}})^2 f^2 [\%] \ (\text{Typical})$$

Loss Tangent Accuracy of $\hat{\mu}_r$ ($\Delta tan\delta$)

Where,
$$\mathbf{E_a} = 0.002 + \frac{0.001}{F \mu'_{\rm rm} f} + 0.004 f$$
 (Typical)

$$\textbf{E}_{\textbf{b}} = \frac{\Delta \mu'_{rm}}{\mu'_{rm}} \frac{tan\delta}{100} \text{ (Typical)}$$

f is measurement frequency [GHz]

$$\mathbf{F} = h \ln \frac{c}{b} [mm]$$

h is the height of MUT [mm]

b is the inner diameter of MUT

c is the outer diameter of MUT

 $tan\delta$ is the measured value of loss tangent

 μ'_{rm} is the measured value of permeability

At the following frequency points, instrument spurious characteristics could occasionally cause measurement errors to exceed specified value.

10.71 MHz 514.645 MHz 17.24 MHz 686.19333 MHz 21.42 MHz 1029.29 MHz 42.84 MHz 1327.38666 MHz

See "EMC" under "Others" in "General Characteristics."

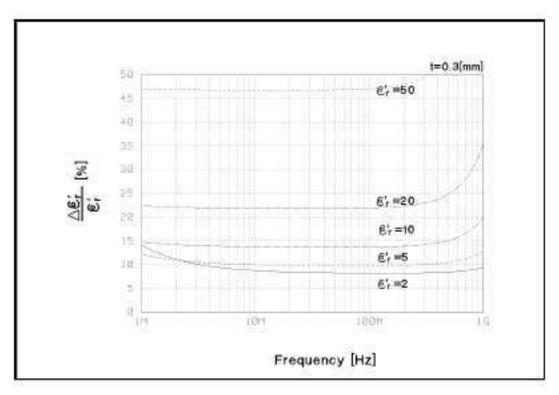


Figure 1-17. Typical Permittivity Measurement Accuracy (@ thickness = 0.3 mm)

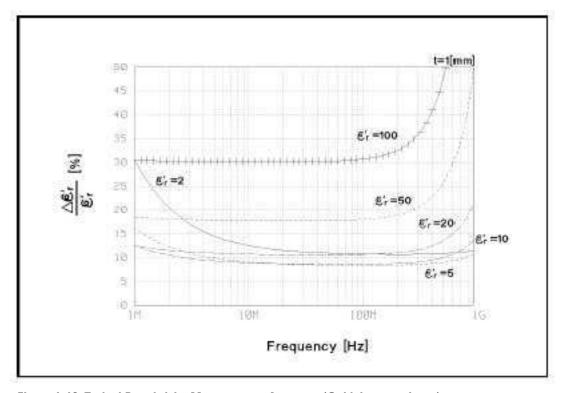


Figure 1-18. Typical Permittivity Measurement Accuracy (@ thickness = 1 mm)

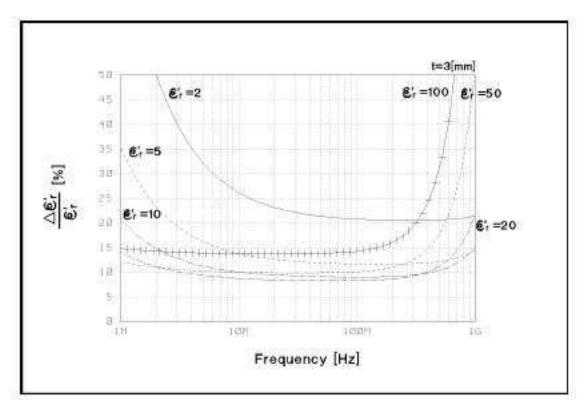


Figure 1-19. Typical Permittivity Measurement Accuracy (@ thickness = 3 mm)

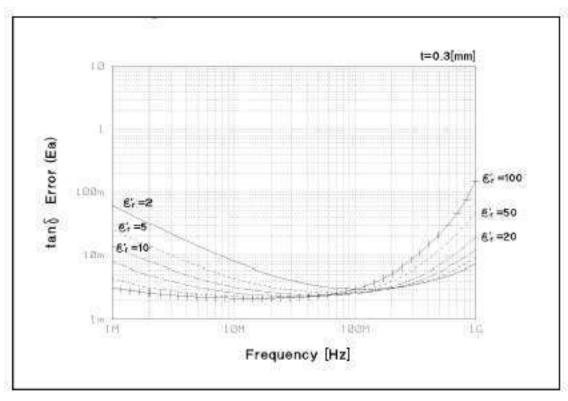


Figure 1-20. Typical Dielectric Loss Tangent ($tan\delta$) Measurement Accuracy (@ thickness = 0.3 mm)

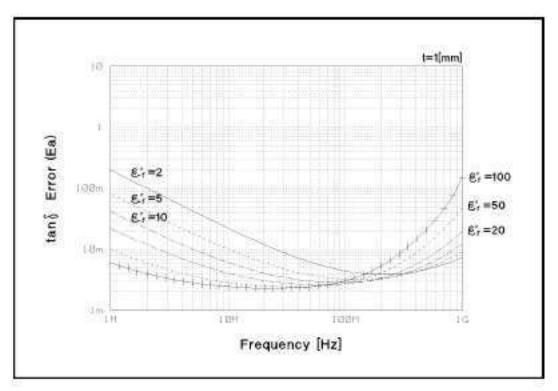


Figure 1-21. Typical Dielectric Loss Tangent ($tan\delta$) Measurement Accuracy (@ thickness = 1 mm)

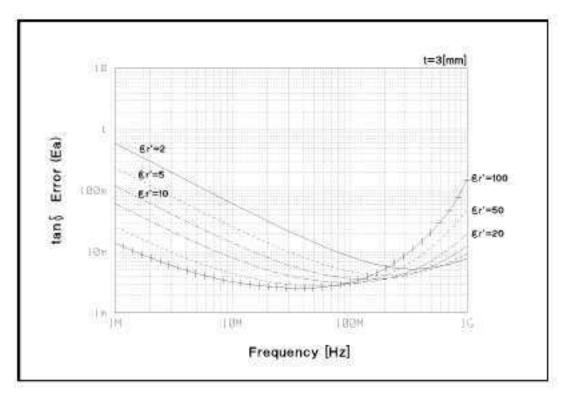


Figure 1-22. Typical Dielectric Loss Tangent ($tan\delta$) Measurement Accuracy (@ thickness = 3 mm)

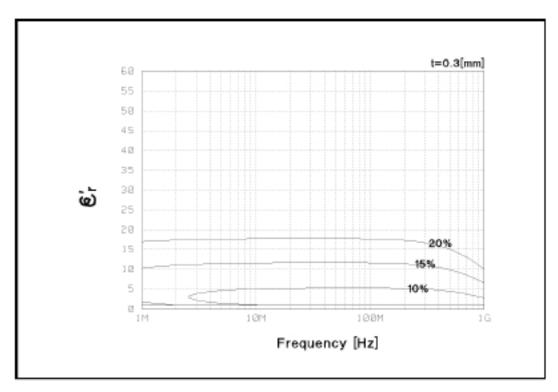


Figure 1-23. Typical Permittivity Measurement Accuracy (ε_r vs. Frequency, @ thickness = 0.3 mm)

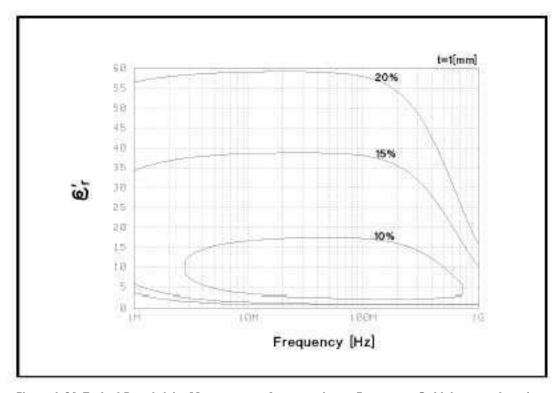


Figure 1-24. Typical Permittivity Measurement Accuracy (ε_r vs. Frequency, @ thickness = 1 mm)

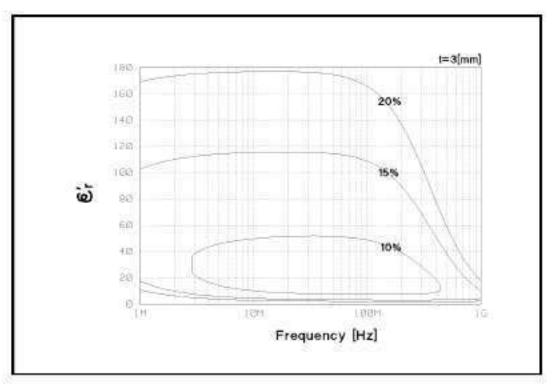


Figure 1-25. Typical Permittivity Measurement Accuracy (ε_r vs. Frequency, @ thickness = 3 mm)

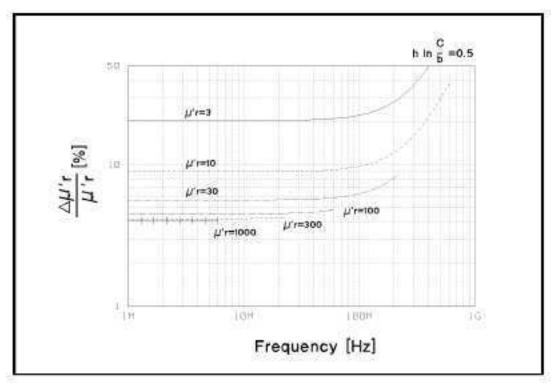
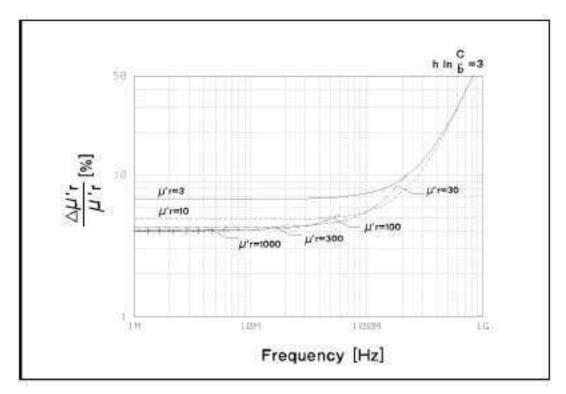


Figure 1-26. Typical Permeability Measurement Accuracy (@ $F^* = 0.5$)



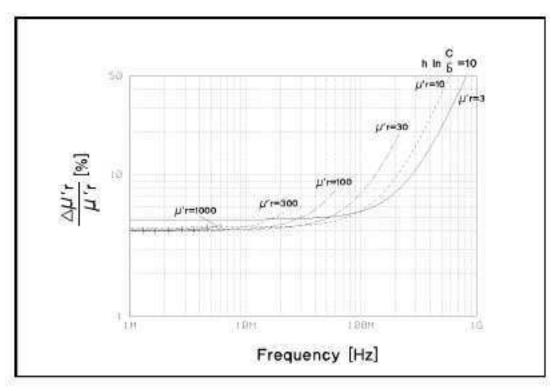


Figure 1-28. Typical Permeability Measurement Accuracy (@ $F^* = 10$)

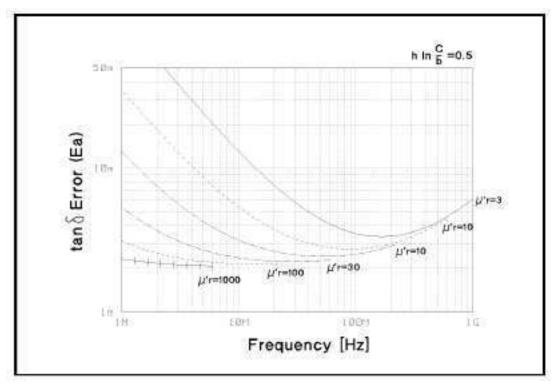


Figure 1-29. Typical Permeability Loss Tangent (tan δ) Measurement Accuracy (@ F* = 0.5) $*_F = h \ln \frac{\sigma}{F}$

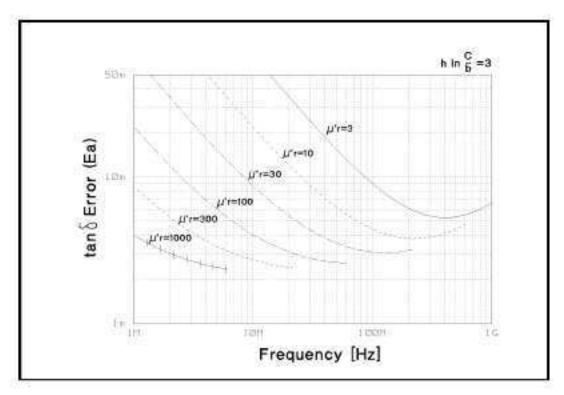


Figure 1-30. Typical Permeability Loss Tangent ($\tan\delta$) Measurement Accuracy (@ F* = 3)

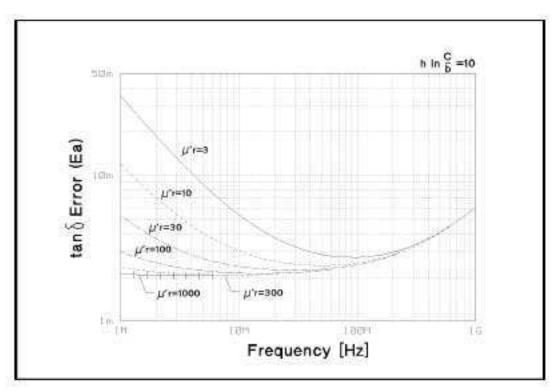


Figure 1-31. Typical Permeability Loss Tangent (tan δ) Measurement Accuracy (@ F* = 10) * = hln $\frac{c}{b}$

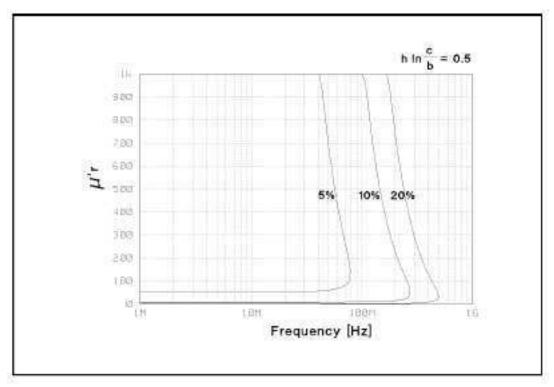


Figure 1-32. Typical Permeability Measurement Accuracy (μ_r vs. Frequency, @ F* = 0.5)

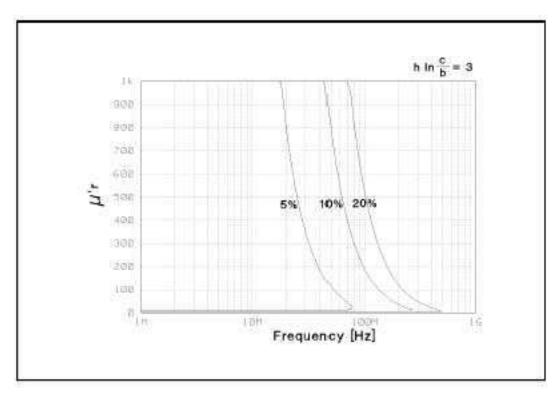


Figure 1-33. Typical Permeability Measurement Accuracy (μ_r vs. Frequency, @ F* = 3) * $_F$ = hln $\frac{c}{b}$

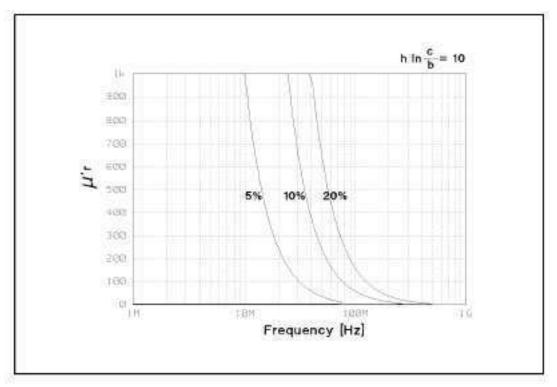


Figure 1-34. Typical Permeability Measurement Accuracy (μ_r vs. Frequency, @ F* = 10) ${}^*F = h \ln \frac{c}{b}$

Applicable MUT (Material Under Test) Size	See Tables 1-5 and 1-6
<u> </u>	
Using the Agilent 16453A	±40 V
Using the Agilent 16454A	±500 mA
Operating Temperature	
Using the Agilent 16453A or 16454A	55°C to +200°C
Operating Humidity	
Wet bulb temperature < 40°C	
Using the Agilent 16453A or 16454A	up to 95% RH

Table 1-5. Applicable Dielectric Material Size Using with the Agilent 16453A





Table 1-6. Applicable Magnetic Material Size Using the Agilent 16454A

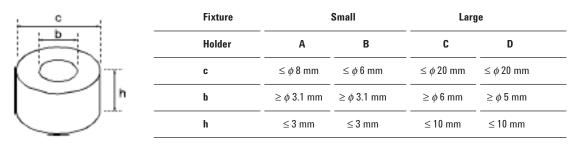

Material Measurement Accuracy with High Temperature Test Head

Option 002 Material Measurement Accuracy with Options 013 and 014 High Temperature Test Head (Typical)

Dielectric Material Measurement Accuracy with High Temperature Test Head (Typical)

Conditions of Dielectric Material Measurement Accuracy with High Temperature Test Head

- Environment temperature is within $\pm 5^{\circ}\mathrm{C}$ of temperature at which calibration is done, and within $0^{\circ}\mathrm{C}$ to $40^{\circ}\mathrm{C}$.
- High Temperature High Impedance Test Head must be used.
- Bending cable should be smooth and the bending angle less than 30°.
- Cable position should be kept in the same position after calibration measurement.
- OPEN/SHORT/50 Ω calibration must be done. Calibration ON.
- Measurement points are same as the calibration points.
- Averaging (on point) factor must be larger than 32 at which calibration is done.
- OSC level must be same as level at which calibration is done.
- OSC level is less than or equal to 0.25 V_{rms} , or greater than 0.25 V_{rms} and frequency range is within 1 MHz to 1 GHz.
- Environment temperature of the main frame is within $\pm 5\,^{\circ}\mathrm{C}$ of temperature at which calibration is done, and within $0\,^{\circ}\mathrm{C}$ to $40\,^{\circ}\mathrm{C}$.

$\epsilon_{\mathbf{r}^{'}}$ Accuracy $(\frac{\Delta\epsilon'_{rm}}{\epsilon'_{rm}}).$	Same as accuracy at which a normal test head is used
	Same as accuracy at which a normal test head is used

At the following frequency points, instrument spurious characteristics could occasionally cause measurement errors to exceed specified value.

10.71 MHz	17.24 MHz	21.42 MHz	42.84 MHz
514.645 MHz	686.19333 MHz	$1029.29 \; \text{MHz}$	1327.38666 MHz

See "EMC" under "Others" in "General Characteristics."

The excessive vibration and shock could occasionally cause measurement errors to exceed specified value.

Typical Effects of Temperature Drift on Dielectric Material Measurement Accuracy

When environment temperature is without $\pm 5^{\circ}\mathrm{C}$ of temperature at which calibration is done, add the following measurement error.

$$\epsilon_{\textbf{r}}' \; \text{Accuracy} \; (\frac{\Delta \epsilon'_{rm}}{\epsilon'_{rm}}) \; \ldots \qquad \qquad \qquad \qquad \\ E_{\epsilon} + \; E_{a3} + \; E_{b3} \, [\%] \; \\$$

Where,

 \mathbf{E}_{ϵ} is ϵ_{r} ' accuracy when a normal test head is used.

 $E_{tan\delta\epsilon}$ is loss tangent accuracy when a normal test head is used.

 E_{a3} is the effect of temperature drift on the accuracy as follows:

$$\mathbf{E_{a3}} = \mathbf{T_c} \Delta \mathbf{T}$$

 E_{b3} is the hysterisis of the effect of temperature drift on the accuracy as follows:

$$\mathbf{E_{b3}} = \underline{\mathbf{T_c}\Delta\mathbf{T}}$$

Where,

 T_c is temperature coefficient as follows:

$$T_c = K_1 + K_2 + K_3$$

$$\mathbf{K}_1 = 1 \times 10^{-6} \times (50 + 300f)$$

$$\mathbf{K_2} = 3 \times 10^{-6} \times (4 + 50f) \left(\frac{\epsilon'_{\text{rm}}}{t} \frac{1}{|1 - (f/f_0)^2|} + 10 \right) f$$

$$\mathbf{K}_{3} = 5 \times 10^{-3} \times (0.2 + 8f^{2}) \frac{1}{(\frac{\varepsilon'_{\text{rm}}}{t} \frac{1}{|1 - (f/f_{0})^{2}|} + 10)f}$$

f: Measurement Frequency [GHz]

$$f_0 = \frac{13}{\sqrt{\varepsilon'_{\rm rm}}} [\text{GHz}]$$

t: Thickness of MUT [mm]

 ϵ'_{rm} : measured value of ϵ'_{r}

The illustrations of temperature coefficient T_c are shown in Figures 1-35 to 1-37.

 ΔT is difference of temperature between measurement condition and calibration measurement condition as follows:

$$\Delta T = |T_{\text{meas}} - T_{\text{cal}}|$$

 T_{meas} : Temperature of Test Head at measurement condition

T_{cal}: Temperature of Test Head at calibration measurement condition

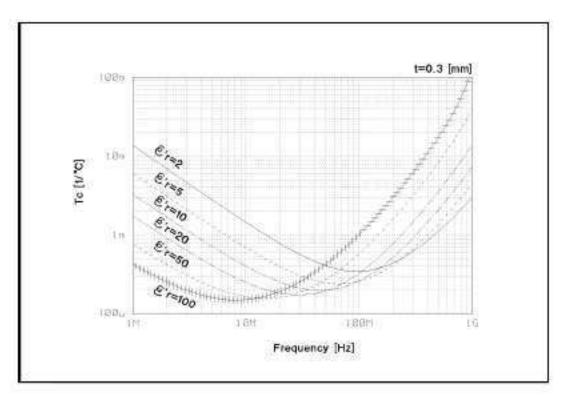


Figure 1-35. Typical Frequency Characteristics of Temperature Coefficient of $\epsilon_{\rm r}'$ and Loss Tangent Accuracy (Thickness = 0.3 mm)

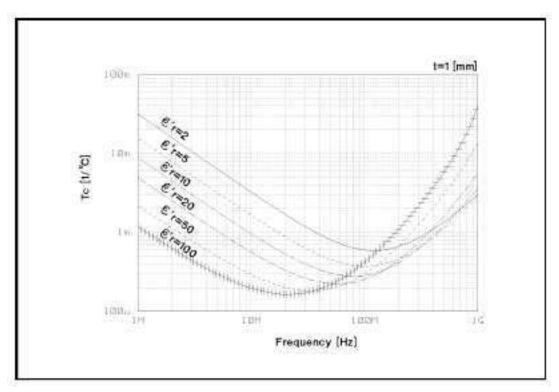


Figure 1-36. Typical Frequency Characteristics of Temperature Coefficient of ϵ_r and Loss Tangent Accuracy (Thickness = 1 mm)

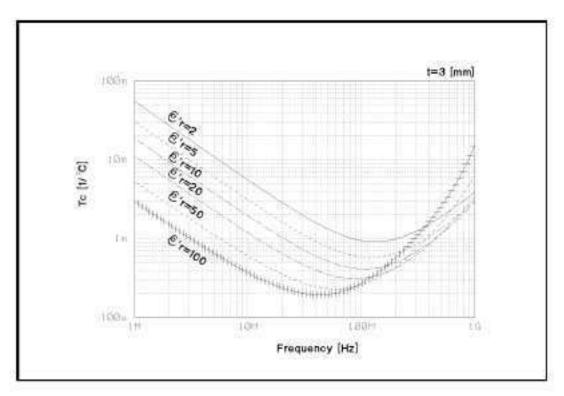


Figure 1-37. Typical Frequency Characteristics of Temperature Coefficient of $\epsilon_{\rm r}'$ and Loss Tangent Accuracy (Thickness = 3 mm)

Material Measurement Accuracy with High Temperature Test Head (Typical) Conditions of Dielectric Material Measurement Accuracy with High Temperature Test Head

- Environment temperature is within ±5°C of temperature at which calibration is done, and within 0°C to 40°C.
- High Temperature Low Impedance Test Head must be used.
- Bending cable should be smooth and the bending angle less than 30°.
- Cable position should be kept in the same position after calibration measurement.
- OPEN/SHORT/50 Ω calibration must be done. Calibration ON.
- · Measurement points are same as the calibration points.
- Averaging (on point) factor must be larger than 32 at which calibration is done.
- OSC level must be same as level at which calibration is done.
- OSC level is less than or equal to 0.25 V_{rms} , or greater than 0.25 V_{rms} and frequency range is within 1 MHz to 1 GHz.
- Environment temperature of the main frame is within ±5°C of temperature at which calibration is done, and within 0°C to 40°C.

Loss Tangent Accuracy of μ_r '($\Delta tan\delta$) Same as accuracy at which a normal test head is used

At the following frequency points, instrument spurious characteristics could occasionally cause measurement errors to exceed specified value.

 10.71 MHz
 17.24 MHz
 21.42 MHz
 42.84 MHz

 514.645 MHz
 686.19333 MHz
 1029.29 MHz
 1327.38666 MHz

See "EMC" under "Others" in "General Characteristics."

The excessive vibration and shock could occasionally cause measurement errors to exceed specified value.

Typical Effects of Temperature Drift on Magnetic Material Measurement Accuracy

When environment temperature exceeds ±5°C of temperature at which calibration is done, add the following measurement error.

$$\mu_{\rm r'} \ {\rm Accuracy} \ (\frac{\Delta \mu'_{\rm rm}}{\mu'_{\rm rm}}) \\ {\rm Loss \ Tangent \ Accuracy \ of \ } \hat{\mu}'_{\rm r} (\Delta \tan \delta) \\ \\ E_{\rm tan \delta \mu} + \ \frac{(E_{\rm a3} + E_{\rm b3})}{100}$$

Where,

 E_{μ} is $\mu'_{\rm r}$ accuracy when a normal test head is used.

 $E_{tan\delta\mu}$ is loss tangent accuracy when a normal test head is used.

 E_{a3} is the effect of temperature drift on the accuracy as follows:

$$\mathbf{E_{a3}} = \mathbf{T_c} \Delta \mathbf{T}$$

 $^*E_{b3}$ is the hysterisis of the effect of temperature drift on the accuracy as follows:

$$\mathbf{E_{b3}} = \underline{\mathbf{T_c}\Delta\mathbf{T}}$$

Where,

 T_c is temperature coefficient as follows:

$$T_c = K_1 + K_2 + K_3$$

$$\mathbf{K_1} = 1 \times 10^{-6} \times (50 + 300f)$$

$$\mathbf{K_2} = 1 \times 10^{-2} \times (1 + 10f^2) \frac{|1 - 0.01\{F(\mu'_{rm} - 1) + 10\}f^2|}{\{F(\mu'_{rm} - 1) + 20\}f} + 10)f$$

$$\mathbf{K_2} = 1 \times 10^{-2} \times (1 + 10f^2) \frac{|1 - 0.01\{F (\mu'_{\rm rm} - 1) + 10\}f^2|}{\{F (\mu'_{\rm rm} - 1) + 20\}f} + 10)f$$

$$\mathbf{K_3} = 2 \times 10^{-6} \times (1 + 30f) \frac{\{F (\mu'_{\rm rm} - 1) + 20\}f}{|1 - 0.01\{F (\mu'_{\rm rm} - 1) + 10\}f^2|}$$

f: Measurement Frequency [GHz]

$$\mathbf{F} = h \ln \underline{\mathbf{c}} [\mathbf{mm}]$$

h is the height of MUT [mm]

b is the inner diameter of MUT

c is the outer diameter of MUT

 $\mu'_{\rm rm}$ is the measured value of permeability

The illustrations of temperature coefficient T_c are shown in Figures 1-38 to 1-40.

ΔT is difference of temperature between measurement condition and calibration measurement condition as follows:

$$\Delta T = |T_{\text{meas}} - T_{\text{cal}}|$$

T_{meas}: Temperature of Test Head at measurement condition

T_{cal}: Temperature of Test Head at calibration measurement condition

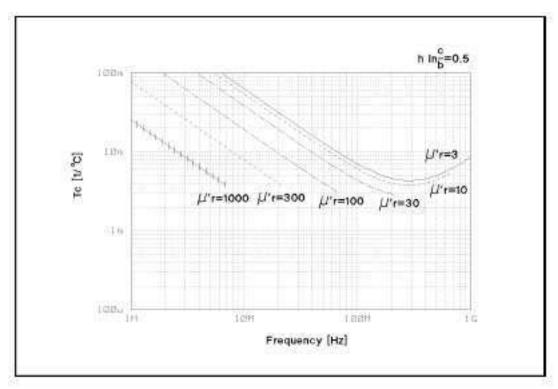


Figure 1-38. Typical Frequency Characteristics of Temperature Coefficient of μ_r ' and Loss Tangent Accuracy (F* = 0.5) $_{^*F}$ = $hln\frac{c}{c}$

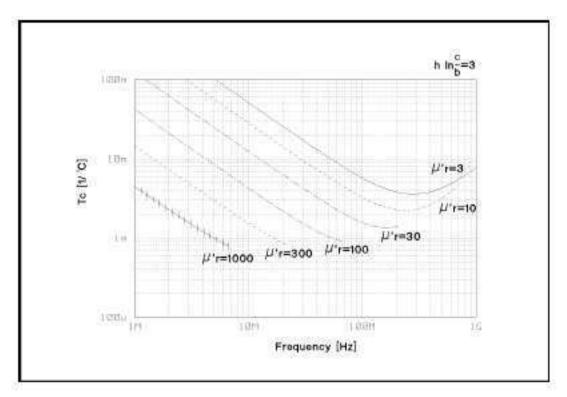


Figure 1-39. Typical Frequency Characteristics of Temperature Coefficient of μ_r ' and Loss Tangent Accuracy (F* = 3) $_{b}^{*}$

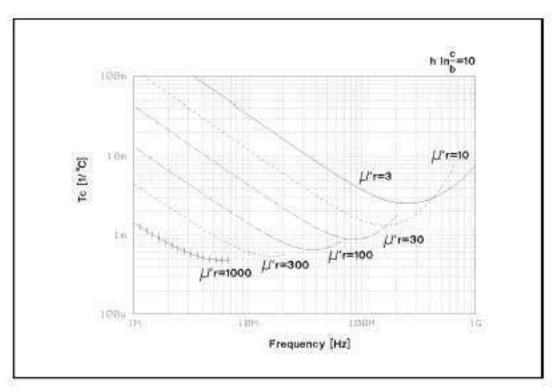


Figure 1-40. Typical Frequency Characteristics of Temperature Coefficient of μ_r ' I and Loss Tangent Accuracy (F* = 10) $^*F = h \ln \frac{c}{b}$

Furnished Accessories

Accessory	Agilent part number
Operating Manual	04291-90020
Programming Manual	04291-90027
Service Manual ¹	04291-90111
Program Disk Set	04291-18000
Power Cable ²	
50 Ω Termination	04291-65006
0 Ω Termination	04191-85300
0 S Termination	04191-85302
Low-Loss Capacitor	04291-60042
Calibration Kit Carrying Case	04291-60041
APC-7 End Cap	16190-25011
Fixture Stand ³	04291-60121
Pad	04291-09001
BNC Adapter⁴	1250-1859
Mini-DIN Keyboard	C3757-60401
Instrument BASIC User's Handbook	E2083-90000
Handle Kit ⁵	5062-3991
Rack Mount Kit ⁸	5062-3979
Rack Mount and Handle Kit ⁷	5062-3985

- 1. Option OBW only
 2. The power cable depends on where the instrument is used; see User's Guide.
 3. Option 013 and 014 only
 4. Option 1D5 only
 5. Option 1CN only
 6. Option 1CM only
 7. Option 1CP only





www.agilent.com/find/emailupdates

Get the latest information on the products and applications you select.



www.agilent.com/find/agilentdirect

Quickly choose and use your test equipment solutions with confidence.



www.agilent.com/find/open

Agilent Open simplifies the process of connecting and programming test systems to help engineers design, validate and manufacture electronic products. Agilent offers open connectivity for a broad range of system-ready instruments, open industry software, PC-standard I/O and global support, which are combined to more easily integrate test system development.

www.agilent.com

Agilent Technologies' Test and Measurement Support, Services, and Assistance

Agilent Technologies aims to maximize the value you receive, while minimizing your risk and problems. We strive to ensure that you get the test and measurement capabilities you paid for and obtain the support you need. Our extensive support resources and services can help you choose the right Agilent products for your applications and apply them successfully. Every instrument and system we sell has a global warranty. Two concepts underlie Agilent's overall support policy: "Our Promise" and "Your Advantage."

Our Promise

Our Promise means your Agilent test and measurement equipment will meet its advertised performance and functionality. When you are choosing new equipment, we will help you with product information, including realistic performance specifications and practical recommendations from experienced test engineers. When you receive your new Agilent equipment, we can help verify that it works properly and help with initial product operation.

Your Advantage

Your Advantage means that Agilent offers a wide range of additional expert test and measurement services, which you can purchase according to your unique technical and business needs. Solve problems efficiently and gain a competitive edge by contracting with us for calibration, extra-cost upgrades, out-of-warranty repairs, and onsite education and training, as well as design, system integration, project management, and other professional engineering services. Experienced Agilent engineers and technicians worldwide can help you maximize your productivity, optimize the return on investment of your Agilent instruments and systems, and obtain dependable measurement accuracy for the life of those products.

United States: Korea: (tel) 800 829 4444 (tel) (080) 769 0800 (fax) 800 829 4433 (fax) (080) 769 0900 Latin America: (tel) 877 894 4414 (tel) (305) 269 7500 (fax) 800 746 4866 Taiwan: (tel) 0800 047 866 China: (tel) 800 810 0189 (fax) 0800 286 331 (fax) 800 820 2816 Other Asia Pacific Europe: Countries: (tel) (65) 6375 8100 (tel) 31 20 547 2111 (fax) (65) 6755 0042 Japan: (tel) (81) 426 56 7832 Email: tm ap@agilent.com (fax) (81) 426 56 7840 Contacts revised: 09/26/05

For more information on Agilent Technologies' products, applications or services, please contact your local Agilent office. The complete list is available at:

www.agilent.com/find/contactus

Product specifications and descriptions in this document subject to change without notice.

© Agilent Technologies, Inc. 1997, 2000, 2006 Printed in USA, July 13, 2006 5966-1543E

