

742A Series

RESISTANCE STANDARDS

Instruction Manual

P/N 850255
September 1988
©1988, John Fluke Mfg. Co., Inc., all rights reserved. Litho in U.S.A.

FLUKE

WARRANTY

John Fluke Mfg. Co., Inc. (Fluke) warrants this instrument to be free from defects in material and workmanship under normal use and service for a period of 1 year from date of shipment. Software is warranted to operate in accordance with its programmed instructions on appropriate Fluke instruments. It is not warranted to be error free. This warranty extends only to the original purchaser and shall not apply to fuses, computer media, batteries or any instrument which, in Fluke's sole opinion, has been subject to misuse, alteration, abuse or abnormal conditions of operation or handling.

Fluke's obligation under this warranty is limited to repair or replacement of an instrument which is returned to an authorized service center within the warranty period and is determined, upon examination by Fluke, to be defective. If Fluke determines that the defect or malfunction has been caused by misuse, alteration, abuse, or abnormal conditions of operation or handling, Fluke will repair the instrument and bill the purchaser for the reasonable cost of repair. If the instrument is not covered by this warranty, Fluke will, if requested by purchaser, submit an estimate of the repair costs before work is started.

To obtain repair service under this warranty purchaser must forward the instrument, (transportation prepaid) and a description of the malfunction to the nearest Fluke Service Center. The instrument shall be repaired at the Service Center or at the factory, at Fluke's option, and returned to purchaser, transportation prepaid. FLUKE ASSUMES NO RISK FOR IN-TRANSIT DAMAGE.

THE FOREGOING WARRANTY IS PURCHASER'S SOLE AND EXCLUSIVE REMEDY AND IS IN LIEU OF ALL OTHER WARRANTIES, EXPRESS OR IMPLIED, INCLUDING BUT NOT LIMITED TO ANY IMPLIED WARRANTY OF MERCHANTABILITY, OR FITNESS FOR ANY PARTICULAR PURPOSE OR USE. FLUKE SHALL NOT BE LIABLE FOR ANY SPECIAL, INDIRECT, INCIDENTAL, OR CONSEQUENTIAL DAMAGES OR LOSS WHETHER IN CONTRACT, TORT, OR OTHERWISE.

CLAIMS

Immediately upon arrival, purchaser shall check the packing container against the enclosed packing list and shall, within thirty (30) days of arrival, give Fluke notice of shortages or any nonconformity with the terms of the order. If purchaser fails to give notice, the delivery shall be deemed to conform with the terms of the order.

The purchaser assumes all risk of loss or damage to instruments upon delivery by Fluke to the carrier. If an instrument is damaged in transit, PURCHASER MUST FILE ALL CLAIMS FOR DAMAGE WITH THE CARRIER to obtain compensation. Upon request by purchaser, Fluke will submit an estimate of the cost to repair shipment damage.

Fluke will be happy to answer all questions to enhance the use of this instrument. Please address your requests or correspondence to: JOHN FLUKE MFG. CO., INC., P.O. BOX C9090, EVERETT, WA 98206,

INTRODUCTION

The 742A Series are small, light, rugged resistance standards. The standards require no temperature-controlled air or oil bath. The 742A Series are well suited for use as the following:

- Working standards
- Portable transfer standards
- Calibration support for the Fluke 5700A Calibrator

Stability and temperature coefficients of the 742A Series make them ideal for easy transport to and operation in any working environment within the range of 18 to 28°C. The standards come with six-month and one-year uncertainty specifications. Depending on the accuracy required, a 742A can be recertified at intervals based on either specification.

Each 742A comes with a Report of Calibration and a rear panel label showing the measured value. The rear panel also has a Fluke Primary Standards Lab calibration label, labels that show temperature coefficient alpha and beta centered on 23°C, and the standard's serial number.

NOTE

Refer to "How Temperature Correction Factors are Calculated," further on in this manual for definitions of alpha and beta.

SPECIFICATIONS

Table 1 lists specifications for the available 742A Series Resistance Standards.

Table 1. 742A Series Resistance Standard Specifications

MODEL	NOMINAL RESISTANCE AT 23°C	TIME STABILITY		CALIBRATION UNCERTAINTY	MAXIMUM DEVIATION FROM THE 23°C VALUE (18 TO 28°C)	MAXIMUM CURRENT (VOLTAGE)	POWER COEFFICIENT +1 PPM WHEN CURRENT EXCEEDS THE FOLLOWING
		180 DAY	1 YEAR				
742A-1	1Ω	±5.0 ppm	±8.0 ppm	±1.0 ppm	3.0 ppm	500 mA (500 mV)	200 mA
742A-10k	10 kΩ	±2.5 ppm	±4.0 ppm	±1.0 ppm	1.5 ppm	3 mA (30V)	0.6 mA

GENERAL SPECIFICATIONS:

Accuracy: The initial resistance is trimmed to ± 2 ppm of nominal. The measured value is printed on the rear panel.

Operating Temperature Range: 23 \pm 5°C

Storage Temperature Range: 0 to 40°C

Report of Calibration: The report of calibration includes a table of resistance values in 0.5° increments from 18 to 28°C.

Size: 8.64 cm H x 10.54 cm W x 12.70 cm L (including binding posts)
(3.4 in H x 4.15 in W x 5.0 in L (including binding posts))
Binding posts; 2.54 cm (1.0 in)

Weight: 0.91 kg (2.0 lbs)

DESIGN AND CONSTRUCTION NOTES

The 742A Series are constructed of arrays of Fluke wirewound precision hermetically-sealed resistors. No adjustable resistors of any kind are used.

Each 742A is built with a temperature coefficient near zero at 23°C. To further reduce errors caused by temperature changes, the binding posts are constructed of low-thermal emf material.

FEATURES

Figure 1 shows a front panel view. Figure 2 shows a rear panel view. Table 2 describes binding post functions. Table 3 describes the rear panel labels.

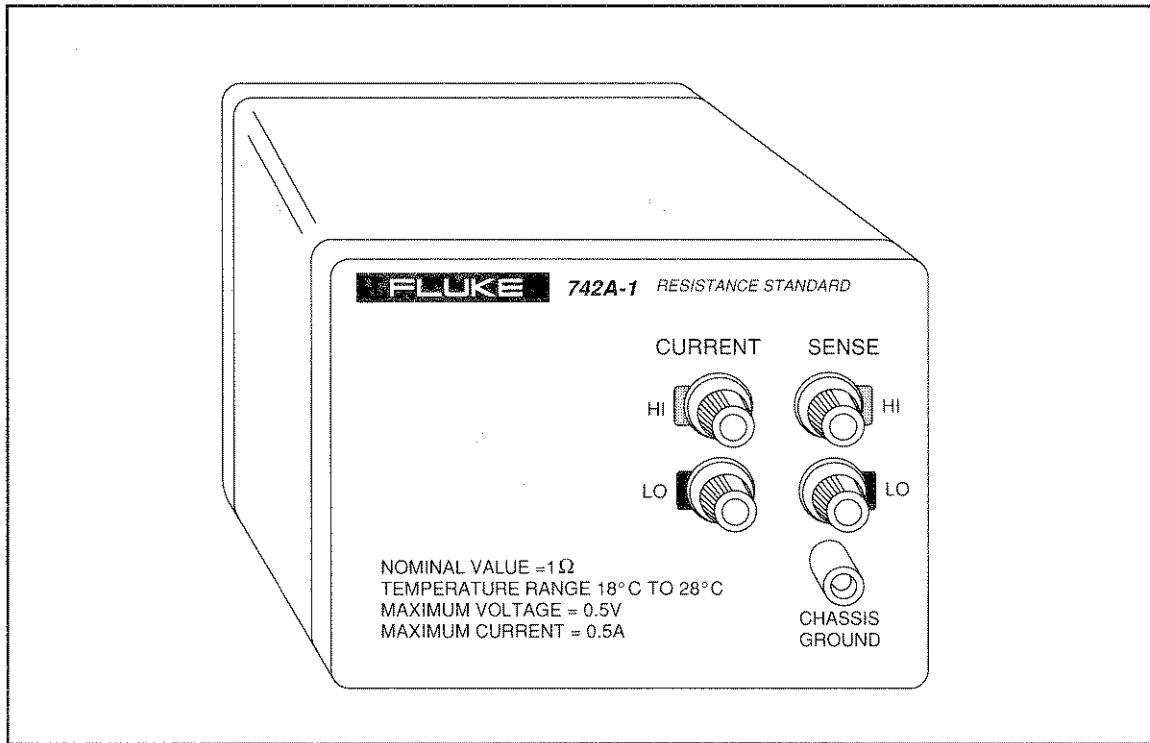


Figure 1. Typical Front Panel View

Table 2. Functions of the Binding Posts

742A BINDING POST	FUNCTION
CURRENT HI	Input for the current source from an ohmmeter
CURRENT LO	Input for the current source from an ohmmeter
SENSE HI	Measurement point for a four-wire ohmmeter
SENSE LO	Measurement point for a four-wire ohmmeter
CHASSIS GROUND	Connected to the case for shielding

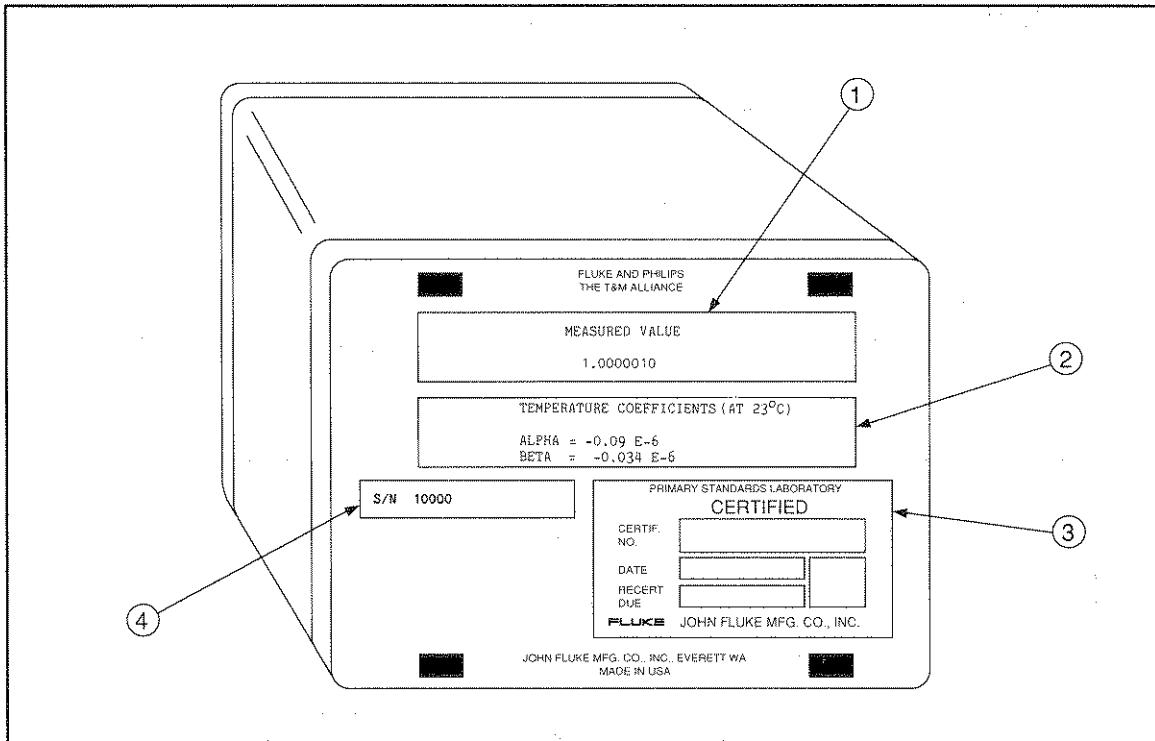


Figure 2. Typical Rear Panel View

Table 3. Contents of the Rear Panel Labels

REF NO.	LABEL INFORMATION
①	Measured value label. Shows the measured value at $23 \pm 0.6^\circ$; the same as on the Report of Calibration.
②	Temperature coefficient label. Shows alpha and beta centered on 23°C . Refer to "How Temperature Correction Factors are Calculated," further on in this manual for definitions of alpha and beta, and the formula to predict exact resistance at different temperatures.
③	Fluke Primary Standards Lab Calibration Label documents traceability to the U.S. National Bureau of Standards.
④	Serial number label. Shows the standard's serial number. This number and the full model number (i.e., 742A-1) positively identify a particular unit.

OPERATING NOTES

This part of the manual explains operational and environmental considerations for the 742A Series. Follow these guidelines when operating or storing the resistance standard. Precautions for handling are under "Care and Maintenance."

Connecting to the 742A Series

CAUTION

Do not apply voltages above the maximum voltage printed on the front panel. Excessive voltage can cause a permanent shift in resistance value or damage.

The specifications for models with CURRENT and SENSE binding posts require four-wire connections to the standard. Use these binding posts as described in Table 2.

For the case to act as a shield, the CHASSIS GROUND binding post must be connected to earth ground or instrument guard at some point in a calibration system. Normally when two or more instruments with guards are connected together, the use of a single common grounding point avoids ground loops. If applicable, ground the 742A CHASSIS GROUND binding post to that common grounding point.

Figure 3 shows a typical connection to a four-wire ohmmeter. Figure 4 shows the connection used to calibrate the 1Ω internal resistance standard in the 5700A.

Cable Recommendations

For optimum results, use two sets of the Fluke 5440A-7004 Low Thermal Test Leads, which are designed to reduce errors caused by thermal emfs.

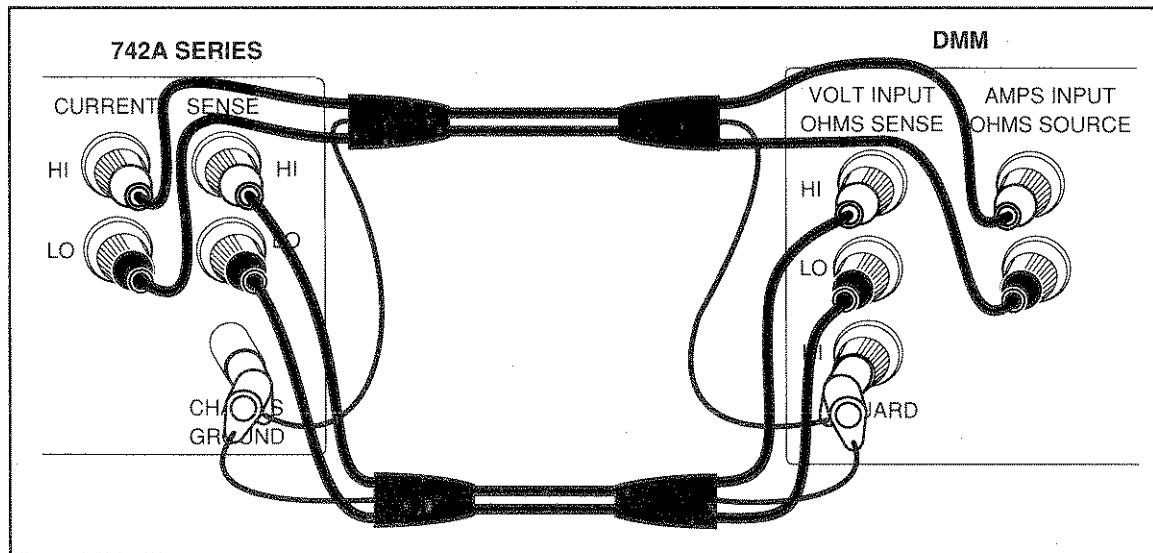


Figure 3. Connection to a Four-Wire Ohmmeter

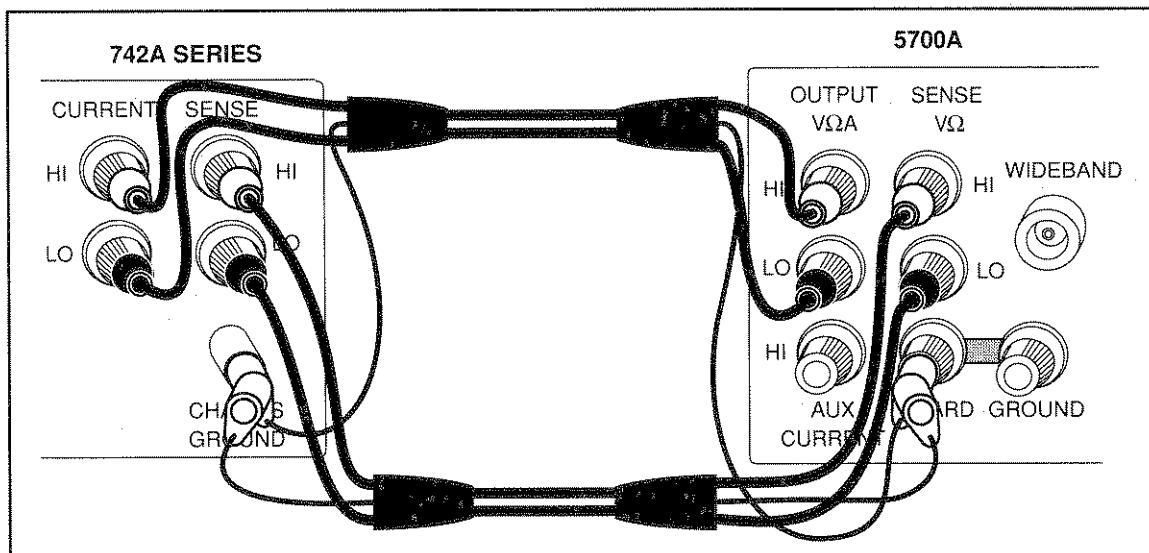


Figure 4. Connection to Calibrate the 5700A

Operating Temperature Range

You can use the 742A Series in ambient temperatures between 18 and 28°C. To predict the deviation from nominal at temperatures other than 23°C, use the temperature characterization table provided with each unit. The table shows the calculated value and the deviation from nominal at temperatures between 18 and 28°C in half-degree increments. An example of this table is included as Table 4.

How Temperature Correction Factors are Calculated

A label on the rear panel shows temperature coefficient factors alpha and beta centered on 23°C. (See Figure 2 for the label location.) The values of alpha and beta are individualized for each 742A. Alpha and beta are established by measurement in the Fluke Primary Standards Lab at 18°C, 23°C, and 28°C. The temperature characterization table is generated from these three measurements and the following formula:

$$R_t = R_{23} [1 + \alpha (t - 23) + \beta (t - 23)^2]$$

Where, R_t = Resistance at $t^{\circ}\text{C}$
 R_{23} = Resistance at 23°C
 α = Slope of the curve (ppm/ $^{\circ}\text{C}$) at 23°C
 β = Rate of change of slope of the curve (ppm/ $^{\circ}\text{C}^2$)

α and β are constants which do not change appreciably over time and hence need to be determined only once.

In the case of the example 742A-1 used in this manual, α and β are calculated as follows:

$$\alpha = \frac{(R_{28} - R_{18})}{\Delta t} = \frac{-0.9 \text{ E-6}}{10} = -0.09 \text{ E-6}$$

$$\beta = \frac{\frac{(R_{28} + R_{18})}{2} - R_{23}}{\left(\frac{\Delta t}{2}\right)^2} = \frac{-0.85 \text{ E-6}}{25} = -0.034 \text{ E-6}$$

Where,
 R_{28} = Resistance at 28°C
 R_{18} = Resistance at 18°C
 R_{23} = Resistance at 23°C
 $\Delta t = (28 - 18) = 10$

Table 4. Example 742A-1 Temperature Characterization Chart

Test Number: XXXX
Date: 04-Aug-88
Page 2 of 2

Serial No.: XXXXXX
Alpha = -0.090 E-6
Beta = -0.034 E-6

Temp (Celsius)	Resistance (OHMS)	Dev from nominal (in ppm)
18.0	1.0000006	0.6
18.5	1.0000007	0.7
19.0	1.0000008	0.8
19.5	1.0000009	0.9
20.0	1.0000010	1.0
20.5	1.0000010	1.0
21.0	1.0000010	1.0
21.5	1.0000011	1.1
22.0	1.0000011	1.1
22.5	1.0000010	1.0
23.0	1.0000010	1.0
23.5	1.0000009	0.9
24.0	1.0000009	0.9
24.5	1.0000008	0.8
25.0	1.0000007	0.7
25.5	1.0000006	0.6
26.0	1.0000004	0.4
26.5	1.0000003	0.3
27.0	1.0000001	0.1
27.5	0.9999999	-0.1
28.0	0.9999997	-0.3

Figure 5 shows a graph of the value of the 742A-1 represented by the sample temperature characterization chart (Table 4). To illustrate use of the formula, calculations for resistance at 20°C and 26°C are shown. You can see that using the formula shown with alpha and beta you get the same value as in the characterization table.

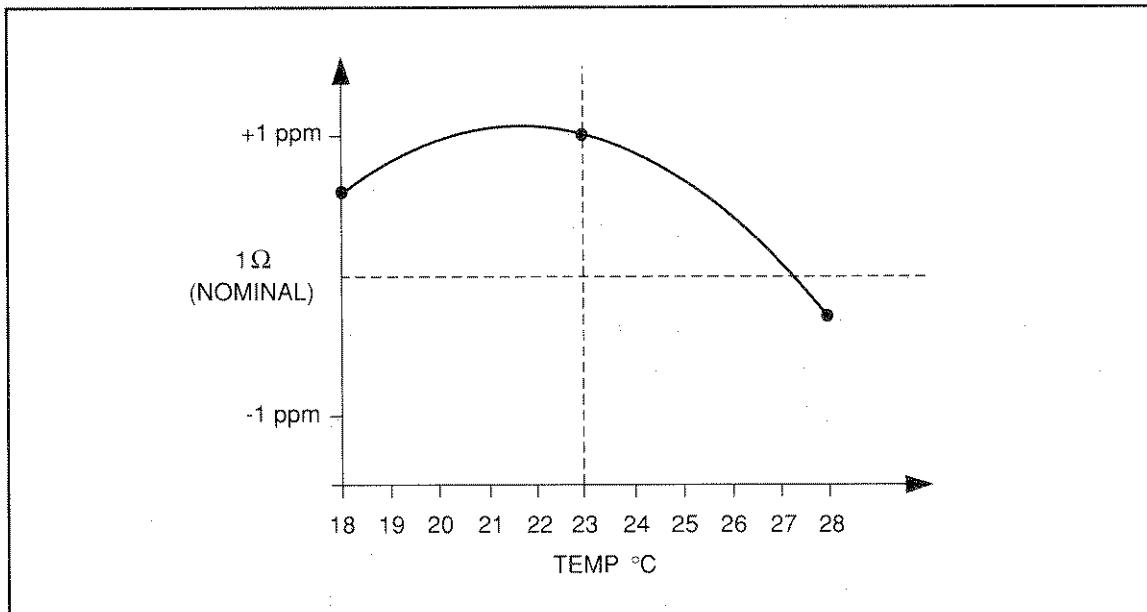


Figure 5. Graph of Resistance VS. Temperature for Sample 742A-1

$$\begin{aligned}
 R_t &= R_{23} [1 + \alpha(t - 23) + \beta(t - 23)^2] \\
 At &= 20^\circ\text{C}, \\
 R_{20} &= 1.0000010 [1 + (-0.09 \times 10^{-6})(-3) + (-0.034 \times 10^{-6})(-3)^2] \\
 &= 1.0000010 (1.0000003 - 0.0000003) \\
 &= 1.0000010 (1.0000000) \\
 &= 1.0000010\Omega
 \end{aligned}$$

$$\begin{aligned}
 R_t &= R_{23} [1 + \alpha(t - 23) + \beta(t - 23)^2] \\
 At &= 26^\circ\text{C}, \\
 R_{26} &= 1.0000010 [1 + (-0.09 \times 10^{-6})(3) + (-0.034 \times 10^{-6})(3)^2] \\
 &= 1.0000010 (1 - 0.0000003 - 0.0000003) \\
 &= 1.0000010 (1 - 0.0000006) \\
 &= 1.0000004\Omega
 \end{aligned}$$

Storage Temperature Range

To maintain accuracy within the specified limits, do not subject the 742A Series to temperatures below 0°C or above 40°C. If exposure to temperatures outside this range is unavoidable, you can minimize the adverse effects by doing the following:

- Keep the standards in the optional transit case (Option 742A-7002). The transit case is insulated and helps protect the standards during short-term temperature extremes.
- Keep exposure to temperature extremes brief.

CARE AND MAINTENANCE

The only maintenance procedure for the 742A Series is occasional cleaning. The following text gives cleaning instructions and precautions for handling.

Cleaning the 742A Series

To keep the 742A Series looking like new, clean the outer surfaces using a soft cloth slightly dampened with water or a non-abrasive mild cleaning solution that does not harm plastics.

CAUTION

Do not use aromatic hydrocarbons or chlorinated solvents for cleaning. They can damage the plastic materials used in the resistance standard.

Precautions for Handling

The 742A Series are designed for mechanical stability, but do not abuse the standard with excessive shock. Avoid temperature extremes as mentioned under "Storage Temperature Range". When you transport the standard, it is recommended that you use the Option 742A-7002 Transit Case for shock and temperature protection. The case holds two 742A Series Resistance Standards.

SERVICING INFORMATION

Because the 742A Series are certified and non-adjustable resistance standards, they are considered non-user repairable. If the unit is damaged, it must be returned to the factory for repair and recalibration.

RECERTIFICATION

For recertification, send the resistance standard to a Fluke technical center. For a nominal fee, Fluke will remeasure and recertify the value of your 742A based on comparison to standards traceable to the U.S. National Bureau of Standards. A new temperature characterization chart is provided on recertification. If you wish, you can record the changes at each recertification and use this data to more closely predict the performance of your 742A. A list of sales and service centers is located near the end of this manual.

Sales and Service Centers

U.S. SALES AREAS for all Fluke products

Alabama

Huntsville
4920 Corporate Drive
Suite J
Huntsville, AL 35805-6202
(205) 837-0581

Arizona

Tempe
2211 S. 48th Street
Suite B
Tempe, AZ 85282
(602) 438-8314

Tucson
(602) 790-9881

California

Burbank
2020 N. Lincoln Street
Burbank, CA 91504
(213) 849-7181

Northern
2300 Walsh Ave., Bldg. K
Santa Clara, CA 95051
(408) 727-0513

San Diego
(619) 292-7657

Southern
P.O. Box 19676
Irvine, CA 92713-9676
16969 Von Karman
Suite 100
Irvine, CA 92714
(714) 863-9031

Colorado

Denver
14180 E. Evans Ave.
Aurora, CO 80014
(303) 695-1000

Connecticut

Hartford
Glen Lochen East
41-C New London Turnpike
Glastonbury, CT 06033
(203) 659-3541

Florida

Clearwater
(813) 799-0087

Miami

(305) 462-1380

Orlando

940 N. Fern Creek Ave.
Orlando, FL 32803
(305) 896-4881

Tampa

(813) 251-9211

Georgia

Atlanta
2700 Delk Road
Suite 150
Marietta, GA 30067
(404) 953-4747

Illinois

Chicago
1150 W. Euclid Avenue
Palatine, IL 60067
(312) 705-0500

Indiana

Indianapolis
8777 Purdue Road
Suite 101
Indianapolis, IN 46268
(317) 875-7870

Louisiana

New Orleans
(504) 455-0814

Massachusetts

Boston
Middlesex Technology Center
900 Middlesex Turnpike
Building 8
Billerica, MA 01821
(617) 663-2400

Maryland

Baltimore
(301) 792-7060

Rockville
5640 Fishers Lane
Rockville, MD 20852
(301) 770-1570

Michigan

Detroit
33031 Schoolcraft
Livonia, MI 48150
(313) 522-9140

Minnesota

Bloomington
1801 E. 79th St.
Suite 9
Bloomington, MN 55420
(612) 854-5526

Missouri

St. Louis
11756 Borman Drive
Suite 160
St. Louis, MO 63146
(314) 993-3805

North Carolina

Greensboro
1310 Beaman Place
Greensboro, NC 27408
(919) 273-1918

New Jersey

Paramus
P.O. Box 930
Paramus, NJ 07653-0930
West 75 Century Road
Paramus, NJ 07652
(201) 262-9550

New Mexico

Albuquerque
(505) 881-3550

New York

Rochester
4515 Culver Road
Rochester, NY 14622
(716) 323-1400

Ohio

Cleveland
Plaza South Three
Suite 402
7271 Engle Road
Middleburg Heights, OH 44130
(216) 234-4540

Oklahoma

Northeast
(405) 236-2977

Oregon

Portland
(503) 227-2042

Pennsylvania

Malvern
200 Lindenwood Drive
Malvern, PA 19355
(215) 647-9550

Pittsburgh
(412) 261-5171

Texas

Austin
(512) 459-3344

Dallas
1801 Royal Lane
Suite 307
Dallas, TX 75229
(214) 869-0311

El Paso
(915) 533-3508

Houston
(713) 240-5995

San Antonio
10417 Gulfdale
San Antonio, TX 78216
(512) 340-0498

Utah

Salt Lake City
(801) 268-9331

Washington

Seattle
5020 148th Ave. N.E.
Suite 110
Redmond, WA 98052
(206) 881-6966

Washington, DC

Washington, DC
(301) 770-1570

INTERNATIONAL SALES OFFICES

Algeria

Bureau de Liaison Philips
 (For Philips products)
 24 rue Bougainville
 El Mouradia, Alger
 Tel: 60 14 05
 TLX: 62221

Antilles

Philips Antillana N.V.
 (For Philips products)
 Schottegatweg Oost 146
 P.O.Box 3523
 Willemstad, Curacao
 Tel: 599-9-615277
 TLX: 1047

Argentina

Coasin S.A.
 (For Fluke products)
 Virrey del Pino 4071DPTO E-65
 1430 CAP FED
 Buenos Aires, Argentina
 Tel: (54) (1) 562-5248
 TLX: (390) 22284

Philips Argentina S.A.
 (For Philips products)
 Casilla Correo 3479
 Vedia 3892
 1430 Buenos Aires
 Tel: 54-1-5414106/5417141
 TLX: 21359/21243

Australia

Elmeasco Instruments Pty, Ltd.
 (For Fluke products)
 P.O. Box 30
 Concord, N.S.W. 2137
 Australia
 Tel: (61) (2) 736-2888
 TLX: (790) AA25887
 FAX: (61) 2-733663

Elmeasco Instruments Pty, Ltd.
 (For Fluke products)
 P.O. Box 623
 12 Maroondah Highway
 Ringwood, Victoria 3134
 Australia
 Tel: (61) (3) 879-2322
 TLX: (790) AA30418
 FAX: (61) 3-879-4310

Elmeasco Instruments Pty, Ltd.
 (For Fluke products)
 P.O. Box 274
 Salisbury, Qld Australia 4107
 Tel: (61) (7) 875-1444
 TLX: (790) AA44062

Elmeasco Instruments Pty, Ltd.
 (For Fluke products)
 P.O. Box 154
 Prospect, South Australia 5082
 Tel: (61) (8) 344-9000

Elmeasco Instruments Pty, Ltd.
 (For Fluke products)
 32 Teddington Rd.
 Victoria Park
 Western Australia 6100
 Tel: (61) 9-470-1855

Philips Scientific & Industrial Equipment Division
 (For Philips products)
 Centrecourt 25-27 Paul Street
 North Ryde
 Sydney N.S.W. 2113
 Tel: 88 88 222

Austria

Walter Rekirsch Elektronische Geräte GmbH & Co.
 (For Fluke products)
 Vertrieb KG
 Obachgasse 28
 1220 Vienna, Austria
 Tel: (43) (222) 253626
 TLX: (847) 134759
 FAX: (43) (222) 257275

Osterreichische Philips Industrie GmbH
 (For Philips products)
 Geschäftsbereich I & E
 Marktbereich Test-und Meßgeräte
 A-1101 WIEN, Triester Straße 64
 Tel: (0222) 60101/1772 DW

Bahrain

Basma W.L.L.
 (For Fluke products)
 P.O. Box 5701
 Manama, Bahrain
 Tel: (973) 251-364
 TLX: (955) 9003
 FAX: (965) 245218

Bangladesh

Motherland Corporation
 (For Fluke products)
 24 Hatkhola Road, Tikatuli
 Dacca-3, Bangladesh
 Tel: 257249, TLX: (950) 642022

Philips Bangladesh Ltd.

(For Philips products)
 P.O. Box 62, Ramna
 16/17 Kawran Bazar C/A
 DHAKA
 Tel: 411976
 TLX: 65668

Belgium

N.V. Philips Professional Systems S.A.
Test and Measurement
 Tweestationsstraat 80
 Rue des Deux Gares
 Brussel 1070 Bruxelles
 Tel: 2-5256111

Bolivia

Coasin Bolivia S.R.L.
 (For Fluke products)
 Casilla 7295
 La Paz, Bolivia
 Tel: (591) (2) 40962
 TLX: (336) 3233 COALAP BV

Brazil

ATP Hi-Tek Eletronica Ltda.
 (For Fluke products)
 Al. Amazonas 422, Alphaville
 Barueri
 CEP 06400, Sao Paulo, Brazil
 Tel: (55) (11) 421-5477
 TLX: (391) 1171413

Philips do Brasil Ltda.

(For Philips products)
 Av. Eng. Luiz Carlos Berrini 3009
 Caixa Postal 8681
 04571 SAO PAULO S.P.
 Tel: 55-11-2411611
 TLX: (011) 32750

Brunei

Rank O'Connor's, Sdn Bhd
 (For Fluke products)
 No. 8 Block D,
 Sufri Shophouse Complex
 Mile 1 Jalan Tutong
 Bandar Seri Begawan
 Negara Brunei Darussalam
 Tel: (673) (2) 23109 or 23557
 TLX: (799) BU2265 RANKOC

Canada

Fluke Electronics Canada Inc.
 400 Britannia Rd. East Unit #1
 Mississauga, Ontario
 L4Z 1X9 Canada
 Tel: (416) 890-7600
 FAX: (416) 890-6866

Fluke Electronics Canada Inc.
 1690 Woodward Drive
 Suite 216
 Ottawa, Ontario
 K2C 3R8 Canada
 Tel: (613) 723-9453
 FAX: (613) 723-9458

Fluke Electronics Canada Inc.
 1255 Trans Canada Highway
 Suite 130
 Dorval, Quebec
 H9P 2V4 Canada
 Tel: (514) 685-0022
 FAX: (514) 685-0039

Chile

Intronica Chile, Ltda.
 (For Fluke products)
 Casilla 16228
 Santiago 9, Chile
 Tel: (56) 2-2321886
 TLX: (332) 346351

Philips Chilena S.A.

de Produc. Electr.
 (For Philips products)
 Avenida Santa Maria 0760
 Casilla 2687
 Santiago De Chile
 Tel: 56-2-770038
 TLX: 240239

China, Peoples Republic of

Fluke International Corp.
 (For Fluke products)
 P.O. Box C9090 M/S 206A
 Everett, WA 98206 U.S.A.
 Tel: (206) 356-5511
 TLX: 185103 FLUKE UT
 FAX: (206) 356-5116

Colombia

Sistemas E Instrumentacion, Ltda.
 (For Fluke products)
 Carrera 13, No. 37-43, Of. 401
 Ap. Aereo 29583
 Bogota DE, Colombia
 Tel: (57) 232-4532
 TLX: (396) 45787

Industrias Philips de Colombia S.A.

(For Philips products)
 Apartado Aereo 4282
 Calle 13 No. 51-39
 Bogota
 Tel: 57-1-2600600
 TLX: Philcolon 44776

Cyprus

Chris Radiovision, Ltd.
 (For Fluke products)
 P.O. Box 1989
 Nicosia, Cyprus
 Tel: (357) (21) 66121
 TLX: (826) 2395

Cyprus, Northern

Ucok Buroteknik
 (For Fluke products)
 2C & 2D Muftu Ziyai Street
 Leikkosa, Northern Cyprus
 Mersin 10, Turkey
 Tel: (90) (741) 357-20-71777
 TLX: (821) 57267

Denmark

Tage Olsen A/S
 (For Fluke products)
 Ballerup Byvej 222
 2750 Ballerup
 Denmark
 Tel: (45) (2) 658111
 TLX: (855) 35293
 FAX: (45) 2-680 300

Philips A/S Test & Measurement
 (For Philips products)
 Prags Boulevard 80
 DK-2300-Kopenhagen S
 Tel: (01) 572222
 TLX: 31201

Ecuador

Proteco Coasin Cia., Ltda.
 (For Fluke products)
 P.O. Box 228-A
 Ave. 12 de Octubre 2285
 y Orellana
 Quito, Ecuador
 Tel: (593) (2) 529684
 TLX: (393) 22085

Philips Ecuador S.A.

(For Philips products)
 Casilla 343
 Paez 118 y Avenida Patria
 Quito
 Tel: 593-2-546100/546125
 TLX: 2227 PHLPSQ ED

Proteco Coasin Cia., Ltda.

(For Fluke products)
 P.O. Box 9733
 Ave. Principal No. 204 y Calle Segunda
 Urbanizacion Miraflores
 Guayaquil, Ecuador
 Tel: (593) (4) 387519

Egypt and Sudan

Electronic Engineering
Liaison Office
 (For Fluke products)
 P.O. Box 2891 Horreya
 11361 Heliopolis, Cairo
 Egypt
 Tel: (20) 2-695705
 TLX: (927) 22782

Philips Egypt Liaison Office of Philips (For Philips products) Export B.V. 10, Abdel Rahman el Rafei Str. P.O. Box 1687 Dokki, Cairo Tel: 20-2-3490922 TLX: 22816 PHEGY UN	Great Britain Philips Test & Measurement York Street Cambridge CB1 2PX Tel: (0223) 358866 TLX: 817331	Hinditron Services Pvt. Ltd. (For Fluke products) 204-5-6 Hemkunt Tower 98 Nehru Place New Delhi, 110019, India Tel: (91) 11-6410380, TLX: (953) 316458	Israel R.D.T. Electronics Engineering Ltd. P.O. Box 43137 Tel Aviv 61430 Israel Tel: (972) (3) 483211, TLX: 371452 FAX: 972-3-492190
Ethiopia (For Philips products) Philips Ethiopia (Priv. Ltd. Co.) Ras Abebe Areguay Avenue P.O. Box 2565 Addis Ababa Tel: 148300	Philips Test & Measurement (For Fluke products) Colonial Way Watford WD2 4TT	Hinditron Services Pvt. Ltd. (For Fluke products) Emerald Complex 1-7-264 5th Floor 114 Sarojini Devi Rd. Secunderabad 500 003, India Tel: 842 821117, TLX: (953) 04256973	Italy Sistrel S.p.A. (For Fluke products) Via Pelizza da Volpedo 59 20092 Cinisello Balsamo Milan, Italy Tel: (39) (2) 6181893, TLX: (843) 334643 FAX: (39) 2-6182440
Fiji Awa New Zealand Ltd. (For Fluke products) 37 Freestone Walu Bay Road P.O. Box 858 Suva, Fiji Tel: (679) 312079 TLX: (792) 2347 FAX: (679) 314379	Greece Hellenic Scientific Representations Ltd. (For Fluke products) 11 Vrassida Street Athens 612, Greece Tel: (30) (1) 7211140 TLX: (863) 219330	Peico Electronics & Electricals Ltd. (For Philips products) Shivsagar Estate, Block 'A' Dr. Annie Besant Road P.O.B. 6598 Worli, Bombay 400018 Tel: 4921500/4921513	Sistrel S.p.A. (For Fluke products) Via le Erminio Spalla No. 41 00142 Rome, Italy TLX: (843) 625857, FAX (39) 6-504137
Finland Instrumentarium Elektronikka (For Fluke products) P.O. Box 64 02631 Espoo 63 Finland Tel: (358) (0) 5281 TLX: (857) 124426 FAX: (358) 0-502-1073	Philips S.A. Hellenique I&E Division (For Philips products) 15, 25th March Street GR-17778 TAVROS or P.O. Box 3153 Athens Tel: 30-1-4894911 TLX: 241566-241567	Indonesia P.T. Lamda Triguna (For Fluke products) Tel: (62) 21-8195365 TLX: (796) 45483 LOMAS I.A. P.O. Box: 6/JATJG, Jakarta 13001	Sistrel S.p.A. (For Fluke products) Via Cintia Parco S. Paolo 35 80126 Naples, Italy Tel: (39) (81) 7679700 FAX (39) 81-7661361
OY Philips AB (For Philips products) P.O. Box 11 02631 ESPOO Tel: 0-5257225	Hong Kong Fluke Asia Ltd. (For Fluke products) Shun Tak Centre Suite No. 1501 200 Connaught Road Central, Hong Kong Tel: (852) 5-482116 FAX: (852) 5-479863 TLX: (780) 87058 Fluke HX	P.T. Daeng Brothers (For Philips products) Centre Point Building, 3rd Fl. Jalan Gatot Subroto Kav. 35/36 P.O. Box 41 Tebet Jakarta Tel: 62-21-517900 TLX: 62798 PHDC IA	Philips S.p.A. (For Philips products) Sezione S & I, T & M Dept. Viale Elvezia 2 20052 Monza Tel: (039) 3635240/8/9 TLX: 333343
France M.B. Electronique S.A. (For Fluke products) 606 Rue Fourney P.O. Box 31 78530 BUC, France Tel: (33) (1) 39568131 TLX: (842) 695414 FAX: (33) (1) 3956-53-44	Philips Hong Kong Ltd. (For Philips products) 29/F Hopewell Centre 17 Kennedy Road G.P.O. Box 2108 Hong Kong Tel: 852-5-283298 TLX: 73660 PHILH HK	Iran Philips Iran Ltd. (For Philips products) (Private Joint Stock Comp.) P.O. Box 11365-3891 Tehran Tel: 98-21-674138 TLX: 212545 PHPS IR	Japan John Fluke Mfg. Co., Inc. Japan Branch (For Fluke products) Sumitomo Higashi Shinbashi Bldg. 1-11 Hamamatsucho Minato-ku, Tokyo 105, Japan Tel: (81) (3) 434-0181 TLX: (781) 2424331 FAX: 81-3-434-0170
S.A. Philips Industrielle et Commerciaux Division Science et Industrie (For Philips products) 105 rue de Paris, BP 62 93002 BOBiGNY Cedex Tel: (1) 49 42 80 80 TLX: 210290	Schmidt & Co (H.K.), Ltd (For Fluke products) 18th Floor, Great Eagle Centre 23 Harbour Road Wanchai, Hong Kong Tel: (852) (5) 8330-222 TLX: (780) 74766 or 76762 FAX: (852) 5-8918754	Iraq Philips Midden Oosten B.V. (For Philips products) Baghdad Branch Hai Al Whida. Area No. 902 Street No. 12, Bldg. 141/10 P.O. Box 5749 Baghdad Tel: 7187181 TLX: 212439 Philips IK	John Fluke Mfg. Co., Inc. Japan Branch (For Fluke products) Katsushige Building 2-45 Kohraibashi Higashi-ku, Osaka 541 Japan Tel: (81) (6) 229-0871 FAX: 81-6-229-1098
Germany Philips GmbH (For Philips products) Unternehmensbereich Elektronik für Wissenschaft und Industrie Vertriebsbereich Testr und Meßtechnik Miramstraße 87 Postfach 310320 D-3500 KASSEL Tel: (0561) 5010. TLX: 997070	India Hinditron Services Pvt. Ltd. (For Fluke products) 69/A.L. Jagmohandas Marg Bombay 400 006, India Tel: (22) 8121316, (91) (22) 8125344 TLX: (953) 1175326	Ireland Circuit Specialists Limited (For Fluke products) Unit 5 Enterprise Centre Plassey Technological Park Casterroy, Limerick Ireland Tel: (852) (61) 330333 TLX: (852) 70092	NF Circuit Design Block Co., Ltd. (For Philips products) 3-20 Tsunashima Higashi, 6-Chome, Kokokuku, Yokohama 223 Tel: (045) 452-0411 TLX: 3823-297
Bereich Fluke Produkts Oskar-Messter-Strape 18 D-8045 Ismaning	Hinditron Services Pvt. Ltd. (For Fluke products) 8th Main Road 33/44A Raj Mahal Vilas Extension Bangalore 560 080, India Tel: (91) 812-363139, TLX: (953) 8452741	P.J. Brennan and Company Ltd. (For Philips products) 61 Stillorgan Industrial Park Stillorgan, Co. Dublin Tel: 952501 TLX: 3817 FAX: 952333	Kenya Philips (Kenya) Ltd. (For Philips products) OL Kalou Road, Industrial Area P.O. Box 30554 Nairobi Tel: 254-2-557999, TLX: 22225 Nairobi

Korea, Republic of Myoung Corporation (For Fluke products) Yeo Eui Do P.O. Box 14 Seoul, Korea Tel: (82) (2) 784-9942 TLX: MYOUNG K24283 FAX (82) 2-784-2387	Somaciel (For Philips products) 304 Boulevard Mohamed V, Casablanca 05 Tel: 30 80 51/52 TLX: 27021	Norsk AI/S Philips (For Philips products) Dept. I&E, Test & Measurement Sandstuveien 70, P.O. Box 1 Manglerud Oslo 6 Tel: 2-680200	Philips Portuguesa, S.A.R.L., Divisao de Sistemas Industriais (For Philips products) e Electri-Acasticc Outurila-Cavimaxille 2795 Linda-A-Velha Tel: 2190071; TLX: 42987
Kuwait Al Bahar International Group (For Fluke products) P.O. Box 26672 Safat 13127 Safat, Kuwait Tel: (965) 848601, TLX: (959) 44822	Nepal Associated Enterprises (For Fluke products) GPO Box 790, Pyaphal Tole Kathmandu, Nepal Tel: 13868, TLX: 2568	Oman OHI Telecommunications (For Fluke products) P.O. Box 889 Muscat, Oman Tel: (968) 603606, TLX: (926) 5052	Saudi Arabia Electronic Equipment Marketing Co. (For Fluke products) P.O. Box 3750 Riyadh, 11481 Saudi Arabia Tel: (928) (1) 477-1650, TLX: 401120
Lebanon and Jordan Mabek (Electronic Division) (For Fluke products) P.O. Box 13-5657 Beirut, Lebanon Tel: 812523, TLX: (923) 22889	Netherlands Philips Nederland Test en Meetapparaten Hoevenseweg 55A 5017 AD TILBURG Postbus 115 5000 AC TILBURG Tel: 013-352455 TLX: 52683	Pakistan International Operations (PAK Private), Ltd. (For Fluke products) 505 Muhammadi House II, Chundrigar Road P.O. Box 5323, Karachi, Pakistan Tel: (21) 221127, TLX: (952) 24494	Singapore, Republic of Rank O'Connor's (PTE) Ltd. (For Fluke products) O'Connor House 98 Pasir Panjang Road Singapore 0511 Republic of Singapore Tel: (65) 4737944, TLX: (786) RS21023
Philips Middle East S.A.R.L. (For Philips products) B.P. 11-670 Ave. Sami Solh Beyrouth Tel: 392320/1 TLX: 20765 LE PHIBAN	Fluke European Headquarters (For Fluke products) P.O. Box 2269 5600 CG Eindhoven The Netherlands Tel: (40) 458045, TLX: (844) 51846 FAX: 31-40-457515	Philips Electrical Co. of Pakistan Ltd. (For Philips products) P.O. Box 7101 M.A. Jinnah Road Karachi 3 Tel: 92-21-725772 TLX: 2874 PHPAK PK	Philips Project Development (S) Pte. Ltd. (For Philips products) Lorong 1, Toa Payoh Singapore 1231, P.O. Box 340 Toa Payoh Central Post Office Singapore 9131 Tel: 65-3502000 TLX: Philips RS/21375
Malaysia Mecomb Malaysia SDN BHD (For Fluke products) P.O. Box 24 46700 Petaling Jaya Selangor, Malaysia Tel: (60) 3-7743422, TLX: (784) MA37764 FAX: (60) 3-774 3414	New Zealand Northrop Instruments & Systems Ltd. (For Fluke products) Information Technology Group 131 Khyber Pass Road Private Bag, Newmarket Auckland 1, New Zealand Tel: (64) (9) 501-801, TLX: (791) 21570 FAX: 64-9-543430	Paraguay Philips del Paraguay S.A. (For Philips products) Avenida Artigas 1519 Casilla de Correo 605 Asuncion Tel: 595-21-291924 TLX: PY 215	South Africa Protea, PNI (For Fluke products) P.O. Box 39127 Bramley 2018 Republic of South Africa Tel: (27) (11) 786-3647 TLX: (960) 4-24409 SA FAX: 27-11-887-1479
Philips Malaysia Snd. Bhd./ Wisma Philips (For Philips products) 1st, 2nd, 3rd Floors, 3 Jalan SS 15/2A, P.O. Box 12163 Subang Jaya 47500 Petaling Jaya Tel: 60-3-7345511 TLX: PHIMAL MA 25111	Northrop Instruments & Systems Ltd. (For Fluke products) Information Technology Group First Floor, Northrop Bldg. 189-191 Willis Street P.O. Box 2406 Wellington, New Zealand Tel: (64) (4) 856-658, TLX: (791) 3380	Peru Importaciones y Representaciones Electronicas S.A. (For Fluke products) Avda. Franklin D. Roosevelt 105 Lima 1, Peru Tel: (51) (14) 28-8650, TLX: (394) 25663	South African Philips (Pty) Ltd. (For Philips products) P.O.B 7703 2 Herb Street New Doornfontein Johannesburg 2000 Tel: (011) 6179111
Malta Fabian Enterprises (For Fluke products) 20, Msida Road Gzira, Malta Tel: 513283/40216, TLX: (638) 1837	Northrop Instruments & Systems Ltd. (For Fluke products) Information Technology Group 110 Mandeville Street P.O. Box 8388 Christchurch, New Zealand Tel: (64) (3) 488-874, TLX: (791) 4801	Philips Peruana S.A. (For Philips products) Av. Alfonso Ugarte 1268 Lima 5 or Apartado 1841 Lima 100 Tel: 51-14-326070 TLX: 21678 PE PHILPER	South Korea Philips Industries (Korea) Ltd. (For Philips products) C.P.O. Box 3680, Philips House 260-199, Itaewon-Dong Yongsan-Ku Seoul Tel: 82-2-794-5011/5 TLX: Philkor K 27291
Mexico Mexicana de Electronica Industrial S.A. (MEXEL) Diagonal No. 27 Entre Calle de Eugenia Y Ave. Colonia del Valle C.P. 03100, Mexico Tel: (905) 660-4323, TLX: (383) 1771038	Philips New Zealand Ltd. Industrial & Electro-acoustic Systems Division 2 Wagnere Place, P.O. Box 4 021 Auckland 3, New Zealand Tel: (09) 894-160 TLX: NZ 2395, FAX: (9) 862-728	Philippines, Republic of Spark Radio & Electronics, Inc. (For Fluke products) Greenhills P.O. Box 610 San Juan, Metro Manila, 3113 Philippines Tel: (2) 775192, TLX: (722 or 732) 27901	Spain ESSA (For Fluke products) Equipos y Sistemas S.A. C/Apolonio Morales, 13-B Madrid 16, Spain Tel: (34) (1) 458-0150, TLX: (831) 42856 FAX: (34) 1-458-0150
Morocco Oussama S.A. (For Fluke products) Angle Boulevard Emile Zola et Rue Rethel P.O. Box 2007 Casa Casablanca, Morocco Tel: (212) 24-13-38, TLX: (933) 22730 M	Nigeria Associated Electronic Products (Nigeria) Ltd. (For Philips products) KM 16, Ikorodu Road, Ojota P.O. Box 1921 Lagos Tel: 234-1-900160/69 TLX: 21961 NG	Philips Industrial Development Inc. (For Philips products) 2246, Pasong Tamo P.O. Box 911 MCCPO Makati Rizal D Metro Manila Tel: 63-2-868951	Philips Iberica S.A.E. Opto (For Philips products) Aparatos de Medida Martinez Villergas 2 Madrid 28027 Tel: 404-2200
	Norway Morgenstierne & Co A/S (For Fluke products) Konghellegate 3 P.O. Box 6688, Rodelokka Oslo 5, Norway Tel: (47) (2) 356110, TLX: (856) 71719 FAX: (47) 2-381457	Portugal Decada Espectral Equipamentos de Electronica (For Fluke products) Av. Bombeiros Voluntarios Lote 102B, Miraflores/Alges 1495 Lisbon, Portugal Tel: (351) (1) 4103420, TLX: (832) 15515 FAX: (351) 1-410-1844	Sri Lanka Computerlink Data Systems, Ltd. (For Fluke products) 331 Union Place Colombo, 2, Sri Lanka Tel: (94) (1) 28641/2, TLX: (954) 22455

Sweden Philips Foersaeljning AB Division Industrielektronik Test & Measurement S-115 84 Stockholm Tel: (08) 782 18 00	Tunisia Selep S.A.R.L. (For Fluke products) 6, Rue de Sparte Tunis - 1000 RP Tunisia Tel: (216) (1) 248093, TLX: (934) 13030	Inds. Venezolanas Philips. S.A. (For Philips products) Av. Francisco de Miranda, Urb. La Carlota, Edf. Centro Empresarial Parque del Este Apartado 1167 Caracas 1010-A Tel: 58-2-203,71111 TLX: 25267 IVPSA VC
Switzerland Traco Electronic AG (For Fluke products) Jenatschstrasse 1 8002 Zurich Switzerland Tel: (41) (1) 201-0711, TLX: (845) 815570	STIET (For Philips products) 32bis rue Ben Ghedahem Tunis Tel: 348666, TLX: 14512	Zaire Philips Electronics S.A.R.L. (For Philips products) 137, Boulevard du 30 juin B.P. 16636 Kinshasa Tel: 31693, TLX: 21078 KINSHASA
Philips AG (For Philips products) Test-und Messtechnik Postfach CH-8027 Zurich Tel. (01) 4882390	Turkey Erkman Elektronik Aletler (For Fluke products) Ticaret Anonim Sirketi Necatibey Cad 92/3 Karakoy, Istanbul, Turkey Tel. (90) (1) 1441546, TLX: (821) 24399 FAX: (90) 1-1497037	Zambia Philips Electrical Zambia Ltd. (For Philips products) Mwembeshi Road P.O. Box 1878 Lusaka Tel: 218511/218701 TLX: ZA 41220
Syria Mabek (Electronics Division) (For Fluke products) P.O. Box 4238 Damascus, Syria	Turk Philips Ticaret A.S. (For Philips products) Inonu Caddesi 78/80 P.K. 504 80074 Beyoglu-Istanbul Tel: 90-1-1435910 TLX: 24192 PHTRTR	Zimbabwe Philips Electrical (Pvt.) Ltd. (For Fluke products) 62 Mutare Road P.O. Box 994 Harare Tel: 47211/48031 TLX: 2236
Philips Moyen-Orient S.A.R.L. (For Philips products) Rue Fardoss 79 P.O. Box 2442 Damascus Tel: 218605/221650 TLX: PHISYR 411203 SY	United Arab Emirates Haris Al-Ataq, Ltd. (For Fluke products) P.O. Box 8141 Kamal Hamza Bldg. Traffic Police Rd. Dubai, U.A.E. Tel: (971) 4-283625, TLX: (958) 48168	For countries not listed above: Philips Export B.V. I&E Export Test & Measuring Building HVW-3 P.O. Box 218 5600 MD Eindhoven The Netherlands Tel: +31 40 324842 TLX: 35000 phtc nl FAX: +31 40 324898
Taiwan Schmidt Electronics Corp. (For Fluke products) 5th Floor, Cathay Min-Sheng Commercial Building, 344 Min-Sheng East Road Taipei 104, Taiwan R.O.C. Tel: (886) (2) 501-3468, TLX: (785) 11111 FAX: (886) 2-5029692	Philips Middle East (For Philips products) Dubai Intern. Trade Centre, 11th Floor P.O. Box 9269 Dubai Tel: 971-4-377000 TLX: 46350 PMOA EM	
Philips Taiwan Ltd. (For Philips products) 150, Tun Hua North Road P.O. Box 22978 Taipei Tel: 886-2-7120500 TLX: 21570 PHILPEI	Al-Sanani Cen. Trad. Est. (For Fluke products) P.O. Box 7187 Abu-Dhabi, U.A.E. Tel: (971) (2) 821370 TLX: (958) 23966	
Tanzania Philips (Tanzania) Ltd. (For Philips products) T.D.F.L. Building - 1st Floor P.O. Box 20104 Ohio/Upanga Rd. Dar es Salaam Tel: 29571/4 TLX: 41016	Uruguay Coasin Uruguay S.A. (For Fluke products) Libertad 2529 Casilla de Correo 1400 Montevideo, Uruguay Tel: (598) (2) 789015, TLX: (398) UY23010	
Thailand Measuretronix Ltd. (For Fluke products) 2102/63 Ramkamhaeng Road Bangkok 10240 Thailand Tel: (66) (2) 374-2516, TLX: (788) 82796	Industrias Philips del Uruguay S.A. (For Philips products) Av. Uruguay 1287 Casilla de Correo 294 Montevideo Tel: 919000 TLX: PHILURU UY 22296	
Philips Electrical Co. of Thailand Ltd. (For Philips products) 283, Silom Road P.O. Box 961 Bangkok 10500 Tel: 66-2-233 6330.9 TLX: 87327 PHILTHA TH	Venezuela Coasin C.A. (For Fluke products) Calle 9 Con Calle 4, Edif Edinurbi Apartado de Correos NR-70.136 Los Ruices Caracas 1070-A, Venezuela Tel: (58) 2-241-0309, TLX: (395) 21027	

TECHNICAL SERVICE CENTERS

U.S. Service Locations

California

Fluke Technical Center
2020 N. Lincoln Street
Burbank, CA 91504
(213) 849-4641

Fluke Technical Center
2300 Walsh Ave., Bldg. K
Santa Clara, CA 95051
(408) 727-8121

Colorado

Fluke Technical Center
14180 East Evans Ave.
Aurora, CO 80014
(303) 695-1000

Florida

Fluke Technical Center
940 N. Fern Creek Avenue
Orlando, FL 32803
(305) 896-4881

Illinois

Fluke Technical Center
1150 W. Euclid Ave.
Palatine, IL 60067
(312) 705-0500

Maryland

Fluke Technical Center
5640 Fishers Lane
Rockville, MD 20852
(301) 770-1576

New Jersey

Fluke Technical Center
West 75 Century Road
P.O. Box 930
Paramus, NJ 07653-0930
(201) 262-9550

Texas

Fluke Technical Center
1801 Royal Lane, Suite 307
Dallas, TX 75229
(214) 869-0311

Washington

Fluke Technical Center
6920 Seaway Blvd.
Everett, WA 98206
(206) 356-5560

International

Argentina

Coasin S.A.
(For Fluke products)
Virrey del Pino 4071
Buenos Aires, Argentina
Tel: 522-5248

Philips Argentina S.A.
(For Philips products)
Cassila Correo 3479
1000 Buenos Aires
Tel: 542-2411/51

Australia

Elmeasco Instruments Pty Ltd.
(For Fluke products)
P.O. Box 30
Concord, N.S.W. 2137
Australia
Tel: 736-2888

Elmeasco Instruments Pty. Ltd.
(For Fluke products)
P.O. Box 623
Ringwood, VIC 3134

Australia
Tel: 879-2322

Elmeasco Instruments Pty. Ltd.
(For Fluke products)
PO Box 274
Salisbury, Queensland 4107
Australia
Tel: 875-1444

Philips Scientific &
Industrial Equip. Div.
(For Philips products)
Centrecourt 25-27 Paul St
North Ryde
Sydney N.S.W. 2113
Tel: 88 88 222

Austria

Walter Rekirsch Elektronische
Geräte GmbH & Co.
(For Fluke products)
Vertrieb KG
Obachgasse 28
1220 Vienna, Austria
Tel: 253626

Oesterreichische Philips
Industrie GmbH
(For Philips products)
Aabteilung Industrie Elektronik
Triesterstrasse 64
A-1100 Wien
Tel: 645521

Algeria

Bureau de Liaison Philips
(For Philips products)
24 bis rue Bougainville
Tl Mouradie, Alger
Tel: 56 56 72

Antillen

Philips Antillana N.V.
(For Philips products)
P.O. Box 523
Willemstad, Curacao
Tel: 414071/74

Bangladesh

Philips Bangla Desh Ltd.
(For Philips products)
P.O. Box 62
Ramna, Dhaka
Tel: 234280

Belgium

N.V. Philips & Mble Assoc
Scientific & Industrial Div
70 Rue des Deux Gares
Brussels, Belgium
Tel: 2-525 6111

Brazil

Hi-Tek Electronica Ltda.
(For Fluke products)
Al. Amazonas 422
Alphaville, Barueri
CEP 06400 Sao Paulo, Brazil
Tel: 421-5477

Industrias Brasileiras
Philips Ltd.
(For Philips products)
Av. Eng. Luiz Carlos Bernini
3009-7 and CEP 04571
Sao Paulo S.P.
Tel: 241.1611

Canada

Fluke Electronics Canada Inc.
400 Britannia Rd
Unit #1
Mississauga, Ontario L4Z 1Y9
Tel: 416-890-7600

Fluke Electronics Canada, Inc.
(For Fluke products)
1255 Trans Canada Highway
Suite 130
Dorval, Quebec H9P 2V4
Tel: 514-685-0022

Fluke Electronics Canada Inc.
(For Fluke products)
101, 1144 29th Ave. N.E.
Calgary, Alberta T2E 7P7
(403) 291-5215

Chile

Intronica Chile Ltda.
(For Fluke products)
Casilla 16228
Santiago 9, Chile
Tel: 2321886

Philips Chilena S.A.
(For Philips products)
Casilla Postal 2687
Santiago de Chile
Tel: 770038

China, Peoples Republic of
Instrimpex - Fluke Service Center
(For Fluke products)
57, Xisi Dong Da Jie
Xicheng-qu
P.O. Box 9085
Beijing

People's Republic of China
Tel: 65-7281

Colombia

Sistemas E Instrumentacion, Ltda
(For Fluke products)
Carrera 13, No. 37-43, Of. 401
Ap. Aereo 29583
Bogota DE, Colombia
Tel: 232-4532

Denmark

Tage Olson A/S
(For Fluke products)
Ballerup, Byveg 222
2750 Ballerup
Denmark
Tel: 658111

Philips Elektronik Systemer A/S
(For Philips products)
Afd. Industri & Forskning
Prags Boulevard 80-P.B. 1919
DK-2300-Koebenhavn S
Tel: 572222

Ecuador

Proteco Coasin Cia., Ltda.
(For Fluke products)
P.O. Box 228-A
Av. 12 de Octubre 2285 y
Orellana
Quito, Ecuador
Tel: 526759

Philips Ecuador S.A
(For Philips products)
Casilla 343
Quito
Tel: 396100

Egypt and Sudan

Electronic Engineering
Liaison Office
(For Fluke products)
P.O. Box 2891 Horreya
11361 Heliopolis
Cairo, Egypt
Tel: 695705

Philips Egypt Branch
of P.M.O.B.V
P.O. Box 1687
10 Abadel Rahman el Rater St
Dokki, Cairo
Tel: 490922

Ethiopia
Philips Ethiopia
(Priv. Ltd. Co.)
(For Philips products)
Ras Aveye Aregau Avenue
P.O. Box 2565
Addis Ababa
Tel: 148300

Finland
Instrumentarium Elektronitka
(For Fluke products)
P.O. Box 64, Viitika 1
02631 ESPOO 63
Finland
Tel: 358-0-5281

OY Philips AB
(For Philips products)
Kaivokatu 8
P.O. Box 255
00101 Helsinki 10
Tel: 1-7271

France
M.B. Electronique S.A.
(For Fluke products)
606, Rue Fourny
P.O. Box 31
78530 BUC, France
Tel: 9568131

S.A. Philips Industrie
et Comerciale
Science et Industry
(For Philips products)
105 Rue de Paris
93002 Bobigny
Tel: 48301111

Norway Morgenstierne & Co. A/S (For Fluke products) Konghellegate 3 P.O. Box 6688, Rodelokka Oslo 5, Norway Tel: 356110	Portugal Decada Espectral (For Fluke products) Equipamentos de Electronica e Cientificos, SARL Av. Bombeiros Voluntarios, Lote 102B Miraflores/Alges 1495 Lisboa, Portugal Tel: 2103420	Philips AG (For Philips products) S & I Equipment Allmendstrasse 140 Postfach 670 CH-8027 Zurich, Switzerland Tel: 488221	United Arab Emirates Philips Middle East b.v. (For Philips products) Dubai Int'l Trade Centre Level 11 P.O. Box 6269 Dubai Tel: 377000
Norsk Akieseiskap Philips Dept. Industry and Telecommunication Sandstuveien 70 P.O. Box 1 Manglerud Oslo 6 Tel: 2-680200	Philips Portuguesa S.A.R.L. (For Philips products) Av. Eng. Duarte pacheco Appartado 1331 Lisbon-1 Tel: (019) 683121	Syria Philips Moyen-Orient S.A. (For Philips products) Rue Fardoss 79 B.P. 2442 Damascus Tel 221650	Uruguay Coasin Uruguay S.A. (For Fluke products) Casilla de Correo 1400 Libertad 2529 Montevideo, Uruguay Tel: 789015
Pakistan Pak International Operations (For Fluke products) 505 Muhammadi House I.I. Chundrigar Road P.O. Box 5323 Karachi Pakistan Tel: 221127/239052	Singapore Rank O'Connor's Singapore (PTE) Ltd. (For Fluke products) 98 Pasir Panjang Road Singapore 0511 Republic of Singapore Tel: 4737944	Taiwan Schmidt Electronics Corp. (For Fluke products) 5th Floor, Cathay Min-Sheng Commercial Building 344 Min-Sheng East Road Taipei, Taiwan, R.O.C. Tel: 5013468	Industrias Philips del Uruguay (For Philips products) Avda Uruguay 1287 Casilla de Correo 294 Montevideo Tel: 915641
Philips Electrical Industries of Pakistan Ltd. (For Philips products) Philips Markaz M.A. Jinnah Road P.O. Box 7101 Karachi 3, Pakistan Tel: 725772/9	Philips Project Development (S) Pte. Ltd. (For Philips products) Lorong 1 Toa Payoh P.O.I Box 340 Singapore 1231 Tel: 2538811	Yung Kang Trading Co. Ltd. (For Philips products) 11th Floor CTS Building 102 Kuang Fu South Road P.O.Box 1467 Taipei Tel: 752-7421	Venezuela Coasin C.A. (For Fluke products) Calle 9 Con Calle 4 Edif. Edinurbi Apartado de Correos Nr-70 136 Los Ruices Caracas 1070-A, Venezuela Tel: 241-0309
Paraguay hilips del Paraguay S.A. (For Philips products) Av. Artigas 1497 Casilla Correo 605 Asuncion Tel 291924	South Africa Fluke S.A. (Pty) Ltd. P.O. Box 39127 Bramley 2018 Republic of South Africa Tel: 786-3647	Philips (Tanzania) Ltd. (For Philips products) P.O. Box 20104 Dar es Salaam Tel: 29571	Industrias Venezolanas Philips S.A. (For Philips products) Av Ppal de los Ruices Apartado Postal 1167 Caracas Tel: 239-3811
Peru Importaciones Y Representaciones Electronicas S.A. (For Philips products) Avda. Franklin D. Roosevelt 105 Lima 1, Peru Tel: 288650	South African Philips (Pty) Ltd. (For Philips products) P.O.B. 7703 2, Herb Street New Doornfontein, Johannesburg 2000 Tel: 786-3647	Thailand Measuretronix Ltd. (For Fluke products) 2102/63 Ramkhamhaeng Rd. Bangkok, 10240 Thailand Tel: 3742516	Zaire S.A.M.E. s.z.r.l. (For Philips products) B.P. 16636 Kinshasa Tel: 31693
Philips Peruana S.A. (For Philips products) Av. Alfonso Ugarte 1268 Apartado 1841 Lima Tel: 32-6070	Spain Equipos Y Sistemas S.A. (ESSA) (For Fluke products) C/Apolonio Morales, 13B Madrid 16, Spain Tel: 4580150	Philips Electrical Company of Thailand Ltd. (For Philips products) Electronic and Communication Systems Dept. 283 Silom Road P.O. Box 961 Bangkok 10 Tel: 233-63330/9	Zambia Philips Electrica Zambia Ltd (For Philips products) Mwembeshi Road P.O. Box 31878 Lusaka Tel: 218511
Philippines Spark Radio and Electronics Corp. (For Fluke products) Greenhills P.O. Box 610 San Juan Metro-Manila Zip, 3113 Philippines Tel: 63-2-775192	Philips Iberica S.A.E. (For Philips products) Dpto Aparatos de Medida Marinez Villergas Z Madrid 28027 Tel: 404-2200	Tunisia S.T.I.E.T. (For Philips products) 32 bis Rue Ben Ghedahem Tunis Tel: 244268	Zimbabwe Philips Electric (Pvt.) Ltd. (For Philips products) P.O. Box 994 62 Umtali Road Beverley, Harare Tel: 47211
Philips Industrial Development Inc. (For Philips products) 2246 Pasong Tamo Makati, Metro Manila Tel: 868951	Sweden Svenska A.B. Philips Div. Industrielektronik Avd. Matinstrument 11584 Stockholm Tel: 782-1800	Turkey Erkman Elektronik Ajetler (For Fluke products) Ticaret Anonim Sirketi Necatibey Cad 92/3 Karakoy, Istanbul, Turkey Tel: 441546	Turk Philips Ticaret A.S. (For Philips products) Posta Kutusu 504 Beykozlu Istanbul Tel: 1435910
	Switzerland Traco Electronic AG (For Philips products) Jenatschstrasse 1 8002 Zurich Switzerland Tel: 2010711		

Germany (F.R.G.) Philips GmbH Unternehmensbereich Elektronik fur Wissenschaft und Industrie Werk fur Messtechnik Oskar-Messter-StraBe 18 8045 Ismaning Deutschland Tel: (089) 96050	Hinditron Services Pvt. Ltd. (For Fluke products) 15 Community Centre Panchshila Park New Delhi, 110 017, India Tel: 6433675	Italy Sistrel S.p.A. (For Fluke products) Via Felizza da Volpedo 59 20092 Cinisello Balsamo Milan, Italy Tel: 6181893	Mexico Mexicana de Electronica Industrial, S.A. (Mexel) (For Fluke products) Diagonal No. 27 Entre Calle de Eugenia Y Ave Colonia del Valle C.P. 03100, Mexico Tel: 660-4323
Great Britain Philips Scientific Test & Measuring Division (For Fluke products) Colonial Way Watford Herts WD2 4TT United Kingdom Tel: 0923-240511	Hinditron Services Pvt. Ltd. Field Service Center (For Fluke products) Emerald Complex 1-7-264 5th Floor 114 Sarojini Devi Road Secunderabad 500 003, India Tel: 821117	Philips S.p.A. (For Philips products) Sezione S & I T & M Dept. Viale Elvezia 2 20052 Monza Tel: (039) 3635.1	Apesa Electronica S.A. de C.V. (For Philips products) Apartado Postal 213 C.P. 50140 Toluca Edo de Mexico
Pye Unicam Ltd. (For Philips products) York Street Cambridge CB1 2PX Tel: 923-40511	Peco Electronic & Electricals Ltd. (For Philips products) Shivsagar Estate Block "A" Dr. Annie Besant Road P.O.B. 6598 Worli, Bombay 400 018 Tel: 4921500	Japan John Fluke Mfg. Co., Inc. Japan Branch (For Fluke products) Sumitomo Higashi Shinbashi Bldg. 1-1-11 Hamamatsucho Minato-ku, Tokyo 105, Japan Tel: 434-0181	Morocco S.A.M.T.E.L. (For Philips products) 2 Rue de Bapaume Casablanca Tel: 243050
Greece Hellenic Scientific Representations Ltd. (For Fluke products) 11 Vrassida Street Athens 612, Greece Tel: 7211140	Indonesia P.T. Lamda Triguna (For Fluke products) P.O. Box 6/JATJG Jakarta 13001, Indonesia Tel: 8195365	Nihon Philips Corporation (For Philips products) Shuwa Shinagawa Building 26-38 Takanawa 3-chrome Minato-ku, Tokyo 108 Tel: 4485511	Netherlands Philips Nederland Test & Meetapparaten (For Fluke products) Hoevenseweg 55A, 5017 AD Tilburg Postbus 115, 5000 AC Tilburg Nederland 35 24 55
Philips S.A. Hellenique (For Philips products) P.O. Box 153 54 Ave Syngrou Athens Tel: 9215311	P.T. Daeng Brothers (For Philips products) Centre Point Bldg - 3rd Floor Jl Jend. Gatot Sugiroto Kav. 35/36 P.O. Box 41 Tebet Jakarta 12950 Tel: 517335	Kenya Philips (Kenya) Ltd. (For Philips products) P.O. Box 30554 Nairobi Tel: 557999	Philips Nederland B.V. (For Philips products) Boschdijk 525 Gebouw VB 5600 MD Eindhoven Tel: 782808
Hong Kong Schmidt & Co (H.K.) Ltd. (For Fluke products) 18th Fl., Great Eagle Centre 23 Harbour Road Wanchai, Hong Kong Tel: 8330-222	Iran Philips Iran Ltd. (For Philips products) P.O.B. 1297 Teheran Tel: 372081/5	Korea Myoung Corporation (For Fluke products) Yeo Eui Do P.O. Box 14 Seoul, Korea Tel: 784-9942	New Zealand Northrop Instruments & Systems Ltd. (For Fluke products) 459 Kyber Pass Road, Private Bag, Newmarket Auckland 1, New Zealand Tel: 501-801
Philips Hong Kong Ltd. (For Philips products) P.O.B. 2108 27-29 Floor Hopewill Centre 17, Kennedy Road Hong Kong Tel: 5-283298	Iraq Philips Iraq W.L.L. (For Philips products) Munir Abbas Building 4th Floor South Gate P.O. Box 5749 Baghdad Tel: 880409	Philips Electronics (Korea) Ltd. (For Philips products) C.P.O. Box 3680 Seoul, Korea Tel: 794-5011/5	Northrop Instruments & Systems Ltd. (For Fluke products) First Floor, Northrop Bldg. 189-191 Willis Street P.O. Box 2406 Wellington, New Zealand Tel: 856-658
Iceland Heimistaeki SF (For Philips products) Saetun 8 Reykjaavik Tel: 24000	Ireland Philips Electrical (Ireland) Ltd. (For Philips products) Newstead Clonskeagh, Dublin 14 Tel: 693355	Lebanon Philips Middle East S.A.R.L. (For Philips products) P.O. Box 11-670 Beirut Tel: 285748/9	Philips Electrical Ind. Ltd. (For Philips products) Scientific & Industrial Div 68-86 Jervois Quay P.O. Box 2097 Wellington C1 Tel: 735735
India Hinditron Services Pvt. Ltd. (For Fluke products) 1st Floor, 17-B, Mahal Industrial Estate Mahakali Road Andheri East Bombay 400 093, India Tel: 6300043	Israel R.D.T. Electronics Engineering Ltd. P.O. Box 43137 Tel Aviv 61430 Israel Tel: 483211	Malaysia Mecomb Malaysia Sdn. Bhd. (For Fluke products) P.O. Box 24 46700 Petaling Jaya Selangor, Malaysia Tel: 774-3422	Nigeria Associated Electronic Products (Nigeria) Ltd. (For Philips products) Km. 16 Ikorodu Road Ojota P.O. Box 1921 Lagos Tel: 932825
Hinditron Services Pvt. Ltd. (For Fluke products) 33/44A Raj Maha Villas Extn. 8th Main Road Bangalore 560 080, India Tel: 363139		Electrnic System (Malaysia) Sdn. Bhd. (For Philips products) Resourse Plaza No. 4 Persianian Barat P.O. Box 12163 Petaling Jaya Selangor, Kuala Lumpru Tel 554511/24	