



**TELEDYNE LECROY**  
Everywhereyoulook™



# Operator's Manual

DXC100A

Differential Probe Pair





**TELEDYNE LECROY**  
Everywhere you look™

© 2013 Teledyne LeCroy, Inc. All rights reserved.

Unauthorized duplication of Teledyne LeCroy documentation materials other than for internal sales and distribution purposes is strictly prohibited. However, clients are encouraged to distribute and duplicate Teledyne LeCroy documentation for their own internal educational purposes.

WaveSurfer, WaveRunner, and Teledyne LeCroy are registered trademarks of Teledyne LeCroy, Inc. Windows is a registered trademark of Microsoft Corporation. Other product or brand names are trademarks or requested trademarks of their respective holders. Information in this publication supersedes all earlier versions. Specifications are subject to change without notice.

## **Warranty**

Teledyne LeCroy warrants this oscilloscope accessory for normal use and operation within specification for a period of one year from the date of shipment. Spare parts, replacement parts and repairs are warranted for 90 days.

In exercising its warranty, Teledyne LeCroy, at its option, will either repair or replace any assembly returned within its warranty period to the Customer Service Department or an authorized service center. However, this will be done only if the product is determined by Teledyne LeCroy's examination to be defective due to workmanship or materials, and the defect is not caused by misuse, neglect, accident, abnormal conditions of operation, or damage resulting from attempted repair or modifications by a non-authorized service facility.

The customer will be responsible for the transportation and insurance charges for the return of products to the service facility. Teledyne LeCroy will return all products under warranty with transportation charges prepaid.

This warranty replaces all other warranties, expressed or implied, including but not limited to any implied warranty of merchantability, fitness or adequacy for any particular purposes or use. Teledyne LeCroy shall not be liable for any special, incidental, or consequential damages, whether in contract or otherwise.

922259-00 Rev A  
February 2013

# Safety Instructions

This section contains instructions that must be observed to keep this oscilloscope accessory operating in a correct and safe condition. You are required to follow generally accepted safety procedures in addition to the precautions specified in this section. **The overall safety of any system incorporating this accessory is the responsibility of the assembler of the system.**

## Symbols

These symbols may appear on the probe body or in this manual to alert you to important safety considerations.



High Voltage, risk of electric shock.



**CAUTION** of potential for damage to probe or instrument it is connected to, or **WARNING** of potential bodily injury. Attend to the accompanying information to protect against personal injury or damage. Do not proceed until conditions are fully understood and met.



**ELECTROSTATIC DISCHARGE (ESD) HAZARD.** Susceptible to damage if anti-static measures are not taken.



**DOUBLE INSULATION**



**PROTECTIVE (EARTH) TERMINAL**

## Precautions

**Connect and disconnect properly.** Connect probe to the measurement instrument before connecting the test leads to a circuit/signal being tested.

**Use only within operational environment listed.** Do not use in wet or explosive atmospheres.

**Use indoors only.**

**Keep product surfaces clean and dry.** Do not submerge probe. Clean with a water- or alcohol-moistened cloth. Do not use harsh or abrasive cleansers.

**Be careful with sharp tips.** Tips may cause bodily injury if not handled properly.

**Do not operate with suspected failures.** Do not use if any part is damaged. Cease operation immediately and sequester the probe from inadvertent use.

## Operating Environment

The accessory is intended for indoor use and should be operated in a clean, dry environment. Before using this product, ensure that its operating environment is maintained within these parameters:

**Temperature:** Operating, 0° to 50° C; Non-operating, -40° to 71° C

**Humidity:** ≤ 80% relative humidity (non-condensing).

**Altitude:** Up to 2000 m (6560 ft).

## Introduction

The DXC100A is a high-performance, matched, passive differential probe pair designed for use with the Teledyne LeCroy DA1855A Differential Amplifiers. The probe pair consists of two well-matched individual probes sharing a common compensation box allowing the attenuation factor on both probes to be simultaneously switched between 10X and 100X. When used with a Teledyne LeCroy DA1885A Differential Amplifier, the probe's attenuation factor is automatically incorporated into the effective gain display and the decimal properly located in the Precision Voltage Generator (PVG) display.

Although primarily designed for use with Teledyne LeCroy amplifiers, the DXC100A can be used with any oscilloscope or plug-in unit with an input impedance of 1 MΩ/15-26pF and one inch (25.4 mm) spacing between connectors.

### A Word about Differential Amplifiers and Probes

When using a differential amplifier it is very important to understand the role probes play in the overall measurement system performance. Probes not only make attachment to the circuit under test more convenient, 10X and 100X attenuating probes also extend the common mode range of the differential amplifier. For example, the DA1855A amplifier has a common mode range of  $\pm 15.5$  volts when the internal attenuators are set to  $\div 1$  and 155 volts when set to  $\div 10$ . The addition of a probe with an attenuation factor of ten extends the common mode range to 1550 volts or the rating of the probe, whichever is less.

However there is a trade-off in that the Common Mode Rejection Ratio (CMRR) capability of even highly matched differential probe pairs seldom matches that of the amplifier. In order to preserve the amplifier's performance at the probe tips, it is important to use probes designed for differential performance. Attempting to use normal 10X or 100X attenuating oscilloscope probes, even high quality probes, results in very poor CMRR performance. Nominally matching X1 probes, however, provide excellent common mode rejection and are recommended.

When making differential measurements, probe compensation is just as important as it is for single-ended measurements. While probe compensation is important, how well the probes are matched is essential. Most probes depend on the accuracy of the oscilloscope's 1 M $\Omega$  input resistor to determine the accuracy of the probe's attenuation factor. Two probes with a 1% accuracy specification can yield a CMRR as low as 50 to 1 at DC while the amplifier CMRR may be higher than 100,000 to 1. At high frequencies, the CMRR is worse.

A differential probe pair must allow for matching at DC as well as over their useful frequency range. Changing the compensation of a differentially matched probe set without following the proper compensation procedure can result in a significant decrease in the CMRR capability of any differential probe pair.

**It is considered good practice to compensate a probe pair for a given amplifier and then keep the probe pair and amplifier together as a system.** Similarly, it is important that once a probe is compensated for a given amplifier, the respective probe always is used on the same input (meaning, one probe always used on the +INPUT and the other always on the -INPUT).

## Probe Grounding

The DXC100A Probe Pair is supplied with accessories allowing for three probe ground connection methods.

In most cases, when the common mode portion of the signal consists mainly of low frequencies (1 MHz and below), the probe ground leads **should not** be connected to the ground of the circuit under test. Instead, they should be connected to each other to minimize the effects of ground loop currents. The signal corruption caused by not having the probes connected to the ground of the circuit under test is common to both inputs and rejected by the differential amplifier.

However, when working in an environment with high RF ambient noise, it is best to connect the probe ground leads to a good RF ground near the point where the signal is being measured.

The best way to determine which probe grounding technique should be used is to try both methods and use the one that provides the least corruption of the differential signal. Probe tip to BNC adapters are required when adjusting the compensation and probe CMRR as they provide the best performance of the three grounding methods.

## Short Calibration Procedure

There are two situations where the Short Calibration Procedure is appropriate:

- When the probe calibration status is unknown or it has been a long time since the probe has been calibrated. A small difference between the two probes can result in a significant CMRR loss, even though the error may be so small that it's irrelevant to transient response. This makes it rather important to occasionally check the CMRR performance of the probes. This can be done by performing **Part 1** and adjusting as needed.
- When critical measurements are required. We recommend checking the DXC100A CMRR by performing at least **Part 1** of the short procedure. When very high slew rate signals ( $>1\text{V/ns}$ ) are encountered, performance can be enhanced over that of a full calibration procedure done with commonly available pulse generators. Notice that the Short Calibration Procedure is the last step in the Full Calibration Procedure.

## DXC100A Differential Probe Pair

---

Once you are accustomed to making these adjustments, they become quick and easy. Part 2 can be attempted when high slew rates ( $>1\text{V/ns}$ ) are encountered, and/or when high frequency (time constraints less than  $20\text{ns}$  and frequencies greater than  $1\text{MHz}$ ) CMRR is especially important.

**Note:** Do not change any of the adjustments associated with the +INPUT. Doing so requires checking the changed adjustment, and perhaps doing the entire Full Calibration Procedure.

Refer to Figure 1, The DXC100A Board Layout for the location of adjustments, and to the schematic diagram in Figure 2, The DXC100A Schematic for guidance. Both figures can be found at the end of this manual.

### Part 1

1. Set the oscilloscope sweep speed to  $10\mu\text{s/div}$ . Connect both probe tips to the same point in the circuit where a measurement is to be made, and set the DA1855A GAIN, ATTENUATOR and INPUT COUPLING controls to the same settings to be used in the measurement. Be sure the signal used does not exceed the maximum common mode voltage allowed (e.g., 155 volts with 10X and DA1855A ATTENUATOR set to X1).
2. Set the DXC100A to 10X. Adjust C8 (-X10 LF) so as to minimize the total deflection.
3. Set the DXC100A to 100X. Adjust C18 (-X100 LF1) so as to minimize the total deflection.

### Part 2

4. Set the oscilloscope sweep speed to  $20\text{ns/div}$ . Now, set the DXC100A ATTENUATION to X10. Adjust R2 (-X10 HF1) and R8 (-X10 HF2) so as to minimize the total deflection.
5. Set the DX100A ATTENUATION to 100X. Adjust R18 (-X100 HF1) so as to minimize the total deflection.



# Full Calibration Procedure

If the probe pair has been repaired or is to be used on a DA1855A other than the one it was originally calibrated with, the probe pair should be calibrated using the following Full Calibration Procedure. The last step is to perform the Short Calibration Procedure as needed for high slew rate signals.

## Required Equipment

Equipment	Description
Differential Amplifier	Teledyne LeCroy Model DA1855A or Equivalent
Oscilloscopes	150 MHz Minimum Bandwidth
Calibration Generator	Tektronix PG506A or Equivalent
DVM	HP 34401A or Equivalent
DC Voltage Generator	HP 6209B or other stable source of 150V and 300V
Probe Tip to BNC Adaptor (2)	Supplied with probes
BNC T Adaptor	Two female and one male BNC connector, no resistors
COAX Cables (2)	50 Ohm
Termination, 50 Ohm	If oscilloscope has no 50 Ohm input impedance
Termination, 75 Ohm	50 Ohm may be substituted
Trimmer Tool	Not supplied with probes

Refer to Figure 1, The DXC100A Board Layout for the location of adjustments, and to the schematic diagram in Figure 2, The DXC100A Schematic for guidance. Both figures can be found at the end of this manual.

1. DA1855A and Oscilloscope Setup

Follow the sequence shown in the previous Short Calibration Procedure topic to set up the DA1855A amplifier with your oscilloscope.

- a. Remove the probe’s bottom cover and attach the probe to the DA1855A.
- b. Turn the entire DA1855A and probe to gain access to the adjustments.

**NOTE:** Do not attach the probe upside down and then reverse the probes after they are compensated. Reversing the probes after they have been compensated results in degradation of CMRR performance.

- c. Set the probes to X10 attenuation.
- d. Initialize the DA1855A to its power-up reset state by turning its power off and then back on.

At this point, the DA1855A is in the following state:

Setting	Status
+Input	Off
-Input	Off
BW Limit	Full
Gain	X1
Attenuator	÷1
Input Resistance	1M
Precision Voltage Generator	+000.00
Comparison or Differential	Comparison
Effective Gain	÷100

- e. Press the ÷1 Attenuator button on the DA1855A. The ÷1 Attenuator light is now on.
- f. Check that the DA1855A Effective Gain indicators change when the probe is switched from 10X to 100X.

IMPORTANT NOTES ABOUT THIS STEP:

- The DXC100A provides probe attenuation factor information to the DA1855A through an 11” black wire which should be plugged into the DA1855A Probe Coding Input jack on the DA1855A rear panel. If the

DA1855A has no probe coding input, and the wire is not used. Skip to Step 2.

- It is important to use the right hardware to connect the probes to the test signals. In all cases, the BNC to probe tip adapters are helpful. For the high frequency adjustments, they are required. CMRR (common mode rejection ratio) adjustments should be done with both probes connected to a BNC T (two female BNC and one male BNC connected together without any matching resistors).
- With the DXC100A connected, let 20 minutes pass to allow the DA1855A to warm up before performing the calibration procedure.

## 2. +Input X10 DC Attenuation

- a. Set the probe to the 10X position.
- b. Connect both probes to the BNC T, the BNC T and the DVM to the dc voltage source.
- c. Set the voltage source to 150 volts.
- d. Press the  $V_{\text{Comp}}$  button. Measure the dc source with DVM and note the actual voltage (e.g. 149.821 volts).
- e. Set the Precision Voltage Generator to equal the noted voltage (e.g. 149.821 volts)<sup>1</sup>
- f. Set the oscilloscope to 10mV/div. Press the +Input DC button.
- g. Set the BW Limit to 20MHz. Press the X10 Gain Button (to invoke AUTOBALANCE).
- h. Adjust R5 (+X10 DC) to bring the DA1855A output to center screen (0 volts) on the oscilloscope. A 1 division error is equivalent to 10mV out of 150 volts, or 0.0067%, or 67 ppm.

## 3. X10 DC CMRR

- a. Continuing from the previous step, press the -Input DC button.

---

<sup>1</sup> When a large voltage is not available, or when extra precision is desired, monitor the PVG output on the DA1855A rear panel and set the PVG to exactly one tenth the voltage applied to the probe. As little as 32 volts may be used to calibrate the +probe using this method. For CMRR, 32 volts is inadequate and a 50 or 60Hz signal of 30 to 90 Vrms is recommended.

## **DXC100A Differential Probe Pair**

---

- b. Adjust R6 (-X10 DC) to bring the DA1855A output to center screen (0 volts) on the oscilloscope. This is a very critical adjustment, and it is desirable to disconnect both probes from the source simultaneously (by removing the BNC T) and observe that the trace stays within 0.25 div (60,000:1 CMRR) between the two conditions.

### **4. +Input X100 DC Attenuation**

- a. Continuing from the previous step, set the probe to the 100X position.
- b. Set the voltage source to 300 volts.
- c. Press the VComp button. Measure DC source with DVM and note the actual voltage (e.g. 302,617).
- d. Set the Precision Voltage Generator to equal the noted voltage (see footnote).
- e. Set the oscilloscope to 10mV/div and 10 $\mu$ s/div.
- f. Press the +Input DC button.
- g. Press the X10 Gain button (to invoke AUTOBALANCE).
- h. Adjust R23 (+X100 DC) to bring the DA1855A output to center screen (0 volts) on the oscilloscope. A 1 division error is equivalent to 100Mv out of 300 V, or 0.03%, OR 330 ppm.

### **5. X100 DC CMRR**

- a. Continuing from the previous step, press the -Input DC button.
- b. Set the oscilloscope to 2mV/div.
- c. Press X10 Gain to invoke AUTOBALANCE.
- d. Adjust R24 (-X100 DC) to bring the DA1855A output to center screen (0 volts) on the oscilloscope. This is a very critical adjustment, and it is desirable to disconnect both probes from the source simultaneously and observe that the trace stays within 0.5 div between the two conditions. 0.5 divisions is equivalent to a CMRR of 30,000:1 (300V/10mV).
- e. Press the +Input Off button.
- f. Press the -Input Off button.
- g. Disconnect both probes and the DVM from the voltage source.

## 6. +Input X10 LF Compensation

**NOTE:** Low frequency compensation of the DXC100A probe attached to the +Input is done by observing a small portion of the large amplitude step. With this magnification, the waveform shows considerable deviation from flat. What is important is that the front (1 $\mu$ s) and rear (about 10ms) of the waveform are at the same level.

- a. Set the probe to the 10X position.
- b. Set the oscilloscope to 10mV/div and 10 $\mu$ s/div.
- c. Terminate the pulse generator's high amplitude output in 50 or (preferable) 75 Ohms, producing approximately a 5 to 8 volt step.
- d. Connect the +probe to the pulse generator's high amplitude output using the probe tip to BNC adaptor.
- e. Press the X10 Gain button (to invoke AUTOBALANCE).
- f. Press the +Input DC button.
- g. Connect the pulse generator's trigger output to the oscilloscope's external trigger input and then trigger the oscilloscope on its external trigger input.
- h. Adjust C7 (+X10LF) so the amplitude at the front of the waveform (1 $\mu$ s) matches the amplitude at the rear of the waveform (10ms using 1ms/div).

## 7. X10 LF CMRR

- a. Continue from the previous step, (using BW Limit set to 20MHz, and the oscilloscope set to 10mV/div and 10 $\mu$ s/div) connect the +probe and – probe to the pulse generator output.
- b. Press the –Input DC button.
- c. Adjust C8 (-X10 LF) capacitor for a minimum amplitude display. The residual displayed amplitude should be less than 5mV peak (10mV p-p at slower sweep speeds where the entire waveform is visible). Ignore the first 1 $\mu$ s after the step (this is adjusted later).

### 8. +Input X10 HF Transient Response

- a. Press the –Input Off button.
- b. Set the BW Limit to Full.
- c. Press the X1 Gain button.
- d. Set the oscilloscope to 20mV/div.
- e. Connect the +probe to the pulse generator's fast rise output using a 50 Ohm termination and the BNC to probe tip adaptor.
- f. Press the  $V_{Diff}$  button to enable  $V_{Diff}$  mode.
- g. Position the trace  $2\frac{1}{2}$  divisions above the centerline using the PVG (-00.500).
- h. Press the +Input DC button.
- i. Set the oscilloscope sweep speed to 10ns/div.
- j. Adjust pulse generator for 5 divisions of a 100kHz signal.
- k. Adjust R1 (+X10 HF1) and R7 (+X10 HF2) for minimum aberrations at the top of the waveform and a system rise time of less than 3.5ns.

### 9. X10 HF CMRR

- a. Continuing from the previous step, disconnect the probe from the pulse generator.
- b. Connect both probes to the pulse generator's fast rise output using a 50 Ohm termination, the BNC T, and two probe tip to BNC adapters.
- c. Disable  $V_{Diff}$  mode by pressing the  $V_{Diff}$  button.
- d. Set the oscilloscope to 5mV/div.
- e. Press the –Input DC button.
- f. Adjust R2 (-X10 HF1) and R8 (-X10 HF2) for minimum displayed signal. The residual displayed amplitude should be less than 15mV (3.0 divisions) peak to peak.

## 10. +Input X100 LF Compensation

**NOTE:** Low frequency compensation of the DXC100A probe attached to the +Input is done by observing a small portion of a large amplitude step. For the 100X probe attenuation, the oscilloscope transient response plays an important part in determining the correct LF compensation adjustment. The oscilloscope response should be measured at this point and recorded as a reference waveform.

The oscilloscope's transient response error may be determined by connecting the oscilloscope to a known flat pulse generator (i.e., Tektronix PG506 fast rise output). Since the DA1855A produces a maximum output of 0.5 volts, apply a waveform that is stepped from -0.5 volts to 0 volts to the oscilloscope. Oscilloscope response is recorded at 10mV/div, 10 $\mu$ s/div. The correct adjustment of the DA1855A produces a waveform most like the recorded reference waveform, and not necessarily the flattest waveform.

Digital oscilloscopes record and store waveforms nicely. Some users of analog oscilloscopes mark waveforms on the CRT face using a grease pencil.

- a. Set the oscilloscope to 10 $\mu$ s/div and 10mV/div.
- b. Press the -Input DC Off button.
- c. Set the probe to the 100X position.
- d. Connect the +probe to the high amplitude output of the pulse generator using a 50 Ohm or (preferably) 75 Ohm termination and the BNC to probe tip adaptor.
- e. Press the X10 Gain button.
- f. Set the pulse generator amplitude to maximums (5-8V peak).
- g. Set the BW Limit to 20 MHz.
- h. Adjust C17 (+X100 LF1) and C11 (+X100 LF2) for a response that matches the oscilloscope response noted earlier. Ignoring any DC offset, the recorded waveform and this displayed trace should match within 0.1 div.

### 11. X100 LF CMRR

- a. Continuing from the previous step, disconnect the probe from the pulse generator.
- b. Connect both probes to the pulse generator's high amplitude output using a 50 Ohm or (preferably) 75 Ohm termination, the BNC T, and two BNC to probe tip adapters.
- c. Press the –Input DC button.
- d. Adjust C18 (-X100 LF1) and C12 (-X100 LF2) for minimum displayed signal. Ignoring the first 1 $\mu$ s (0.1div), the residual displayed amplitude should be less than 2mV (0.2div) peak to peak.

### 12. +Input X100 HF Transient Response

- a. Press the –Input Off button.
- b. Press the X10 Gain button.
- c. Set BW Limit to Full. Set the oscilloscope to 20mV/div.
- d. Connect the +probe to the pulse generator's fast rise output using a 50 Ohm termination and the BNC to probe tip adaptor.
- e. Press the VDiff button to enable VDiff mode.
- f. Position the trace 2.5 divisions above the centerline using the PVG (-00.500).
- g. Press the +Input DC button.
- h. Set the oscilloscope sweep speed to 10ns/div. Adjust pulse generator for 5 divisions of a 100 kHz signal.
- i. Adjust R17 (X100 HF) for minimum aberrations at the top of the waveform and a system rise time of less than 3.5ns.

### 13. X100 HF CMRR

- a. Continuing from the previous step, disconnect the probe from the pulse generator.
- b. Connect both probes to the pulse generator's fast rise output using a 50 Ohm termination, the BNC T, and two probe tips to BNC adapters.
- c. Disable VDiff mode by pressing the VDiff button.



- d. Set the oscilloscope to 5mV/div.
- e. Adjust R18 (-X100 HF1) for minimum displayed signal. The residual displayed amplitude should be less than 8mV peak to peak (1.6 div).
- f. Now, replace probe cover. Replacing the probe cover disturbs the X10 LF and X100 LF compensations for CMRR very slightly. These fine adjustments need to be made now.

## 14. Final Adjustments and Notes

- a. Set the BW Limit to 20MHz.
- b. Set the oscilloscope to 10mV/div and 10 $\mu$ s/div, and the probe attenuation to 10X.
- c. Terminate the pulse generator's high amplitude output in 50 or (preferably) 75 Ohms, producing approximately a 5 to 8 volt step.
- d. Connect both probes to the pulse generator's high amplitude output using the BNC T and two probe tips to BNC adaptors.
- e. Press the X1 Gain button.
- f. Press the +Input and -Input DC buttons.
- g. Adjust C8 (-X10 LF) capacitor for a minimum amplitude display. Ignoring the first 1 $\mu$ s, the residual displayed amplitude should be less than 5mV peak to peak.
- h. Continuing from the previous step now set the probe attenuation to 100X.
- i. Adjust C18 (-X100 LF1) capacitor for a minimum amplitude display.

**NOTE:** Pulse generators such as the Tektronix PG506 (that do not have a high enough slew rate) may be encountered in some measurement situations. Therefore it is reasonable to make minor adjustments to the -probe compensation to improve the CMRR using a specific source. Do this by connecting both probes to a suitable test point in the circuit under test and adjusting the C8 (-X10 LF), R2 (-X10 HF1), R8 (-X10 HF2) or C18 (-X100 LF1), and R18 (-X100 HF1) as needed. This is the same as performing the DXC100A Probe Short Calibration Procedure.

# DXC100A Differential Probe Pair

When the +probe has been properly adjusted it should be used as a reference. CMRR adjustments made to the probe in the future should be done to the – probe.

**At this point, do not change any of the +Input X10 or +Input X100 Adjustments,** as doing so may require repeating the entire probe calibration procedure.

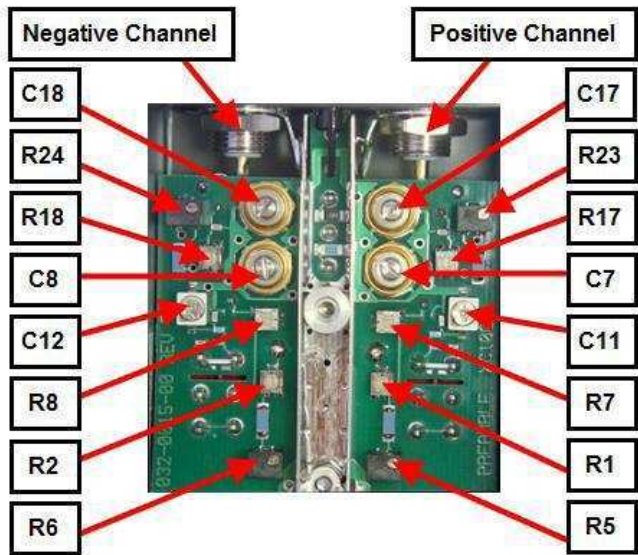


Figure 1, The DXC100A Board Layout

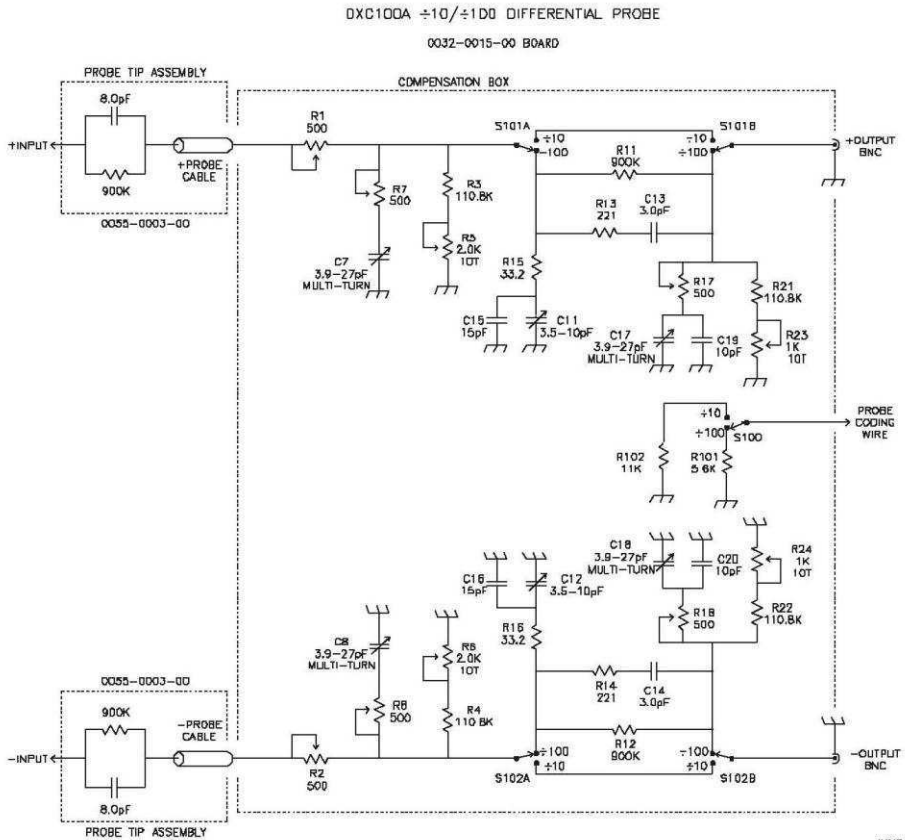


Figure 2, The DXC100A Schematic

JUNE 8, 2001

# Certifications

This section contains the instrument's Electromagnetic Compatibility (EMC), Safety and Environmental certifications.

## EMC Compliance

### EC Declaration of Conformity - EMC

The probe meets intent of EC Directive 2004/108/EC for Electromagnetic Compatibility. Compliance was demonstrated to the following specifications as listed in the Official Journal of the European Communities:

EN 61326-1:2006, EN 61326-2-1:2006 EMC requirements for electrical equipment for measurement, control, and laboratory use.

#### ***Electromagnetic Emissions:***

CISPR 11:2003, Radiated and Conducted Emissions Group 1, Class A <sup>1 2</sup>

#### ***Electromagnetic Immunity:***

EN 61000-4-2:2001 Electrostatic Discharge, 4 kV contact, 8 kV air, 4 kV vertical/horizontal coupling planes <sup>3</sup>

EN 61000-4-3:2006 RF Radiated Electromagnetic Field, 3 V/m, 80-1000 MHz; 3 V/m, 1400 MHz - 2 GHz; 1 V/m, 2 GHz - 2.7 GHz <sup>3</sup>

1 Emissions which exceed the levels required by this standard may occur when the probe is connected to a test object.

2 This product is intended for use in nonresidential areas only. Use in residential areas may cause electromagnetic interference.

3 Meets Performance Criteria "B" limits of the respective standard: during the disturbance, product undergoes a temporary degradation or loss of function or performance which is self-recoverable.

#### ***European Contact:***

Teledyne LeCroy Europe GmbH  
Waldhofer Str 104  
D-69123 Heidelberg  
Germany  
Tel: (49) 6221 82700

### Australia & New Zealand Declaration of Conformity—EMC

Probe complies with the EMC provision of the Radio Communications Act per the following standards, in accordance with requirements imposed by Australian Communication and Media Authority (ACMA):

CISPR 11:2003 Radiated and Conducted Emissions, Group 1, Class A, in accordance with EN61326-1:2006 and EN61326-2-1:2006.

#### **Australia / New Zealand Contacts:**

Vicom Australia Ltd.  
1064 Centre Road  
Oakleigh, South Victoria 3167  
Australia

Vicom New Zealand Ltd.  
60 Grafton Road  
Auckland  
New Zealand

### Safety Compliance

#### **EC Declaration of Conformity – Low Voltage**

The probe meets intent of EC Directive 2006/95/EC for Product Safety. Compliance was demonstrated to the following specifications as listed in the Official Journal of the European Communities:

EN 61010-031/A1:2008 Safety requirements for electrical equipment for measurement, control, and laboratory use – Part 031: Safety requirements for hand-held probe assemblies for electrical measurement and test.

### Environmental Compliance

#### **End-Of-Life Handling**



The instrument is marked with this symbol to indicate that it complies with the applicable European Union requirements to Directives 2002/96/EC and 2006/66/EC on Waste Electrical and Electronic Equipment (WEEE) and Batteries.

The instrument is subject to disposal and recycling regulations that vary by country and region. Many countries prohibit the disposal of waste electronic equipment in standard waste receptacles. For more information about proper disposal and recycling of your Teledyne LeCroy product, please visit [teledynelecroy.com/recycle](http://teledynelecroy.com/recycle).

#### **Restriction of Hazardous Substances (RoHS)**

This instrument has been classified as Industrial Monitoring and Control Equipment and is outside the scope of the 2011/65/EU RoHS Directive until 22 July 2017 (per Article 4, Paragraph 3).

# Contact Teledyne LeCroy

### Teledyne LeCroy Service Centers

#### **United States and Canada - World Wide Corporate Office**

Teledyne LeCroy Corporation  
700 Chestnut Ridge Road  
Chestnut Ridge, NY, 10977-6499, USA  
Ph: 800-553-2769 / 845-425-2000  
FAX: 845-578-5985

teledynelecroy.com

#### **Support:**

contact.corp@teledynelecroy.com

#### **Sales:**

customersupport@teledynelecroy.com

#### **United States - Protocol Solutions Group**

Teledyne LeCroy Corporation  
3385 Scott Boulevard  
Santa Clara, CA, 95054, USA  
FAX: 408-727-0800  
teledynelecroy.com

#### **Sales and Service:**

Ph: 800-909-7211 / 408-727-6600  
contact.corp@teledynelecroy.com

#### **Support:**

Ph: 800-909-7112 / 408-653-1260  
psgsupport@teledynelecroy.com

#### **European Headquarters**

Teledyne LeCroy SA  
4, Rue Moïse Marcinhes  
Case postale 341  
1217 Meyrin 1  
Geneva, Switzerland  
Ph: + 41 22 719 2228 / 2323 / 2277  
FAX: +41 22 719 2233  
contact.sa@teledynelecroy.com  
applications.indirect@teledynelecroy.com  
teledynelecroy.com/europe

#### **Protocol Analyzers:**

Ph: +44 12 765 03971

#### **Singapore, Oscilloscopes**

Teledyne LeCroy Singapore Pte Ltd.  
Blk 750C Chai Chee Road #02-08  
Technopark @ Chai Chee  
Singapore 469003  
Ph: ++ 65 64424880  
FAX: ++ 65 64427811

#### **Singapore, Protocol Analyzers**

Genetron Singapore Pte Ltd.  
37 Kallang Pudding Road, #08-08  
Tong Lee Building Block B  
Singapore 349315  
Ph: ++ 65 9760-4682

#### **China**

Teledyne LeCroy Corporation Beijing  
Rm. 2001 - Office; Rm. 2002 - Service Center  
Unit A, Horizon Plaza  
No. 6, Zhichun Road, Haidian District  
Beijing 100088, China  
Ph: ++86 10 8280 0318 / 0319 / 0320  
FAX: ++86 10 8280 0316

#### **Service:**

Rm. 2002  
Ph: ++86 10 8280 0245

#### **Korea**

Teledyne LeCroy Korea  
10th fl. Ildong Bldg.  
968-5 Daechi-dong, Gangnam-gu  
Seoul 135-280, Korea  
Ph: ++ 82 2 3452 0400  
FAX: ++ 82 2 3452 0490

#### **Taiwan**

LeColn Technology Co Ltd.  
Far East Century Park, C3, 9F  
No. 2, Chien-8th Road,  
Chung-Ho Dist., New Taipei City, Taiwan  
Ph: ++ 886 2 8226 1366  
FAX: ++ 886 2 8226 1368

#### **Japan**

Teledyne LeCroy Japan  
Hobunsya Funchu Bldg, 3F  
3-11-5, Midori-cho, Fuchu-Shi  
Tokyo 183-0006, Japan  
Ph: ++ 81 4 2402 9400  
FAX: ++ 81 4 2402 9586  
teledynelecroy.com/japan





**TELEDYNE LECROY**  
Everywhere**you**look™

700 Chestnut Ridge Road  
Chestnut Ridge, NY 10977  
USA

[teledynelecroy.com](http://teledynelecroy.com)

[www.valuetronics.com](http://www.valuetronics.com)